

Sample Information

Sample Name :Dermaseptin
 Cat No :RP11228
 Lot No :PE6261802

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

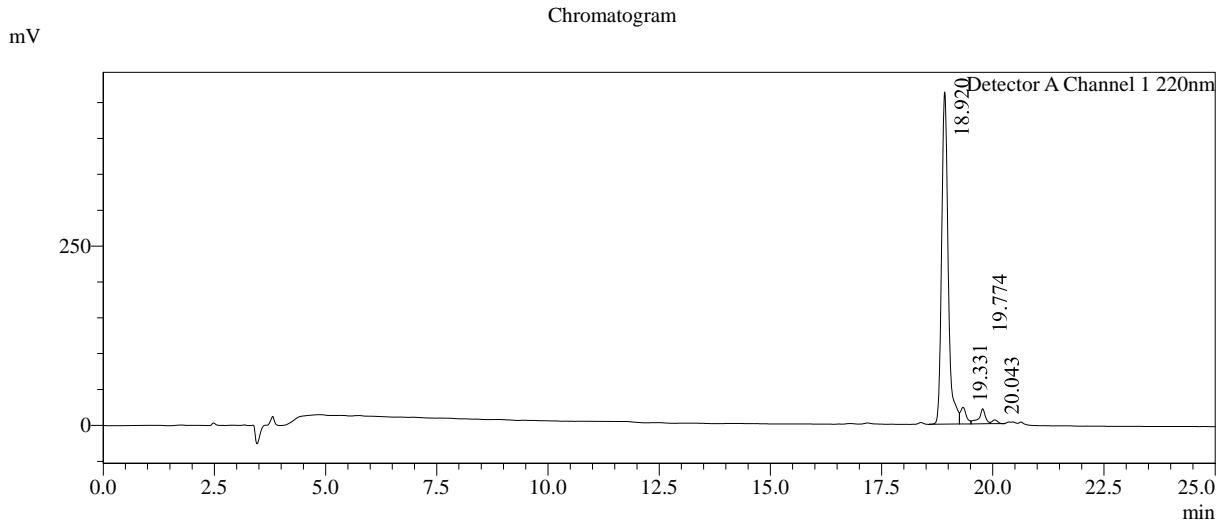

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	18.920	463065	4727917	90.382	90.911
2	19.331	23171	213047	4.522	4.097
3	19.774	20887	214831	4.077	4.131
4	20.043	5220	44822	1.019	0.862
Total		512343	5200617	100.000	100.000