


Mass Spectrum

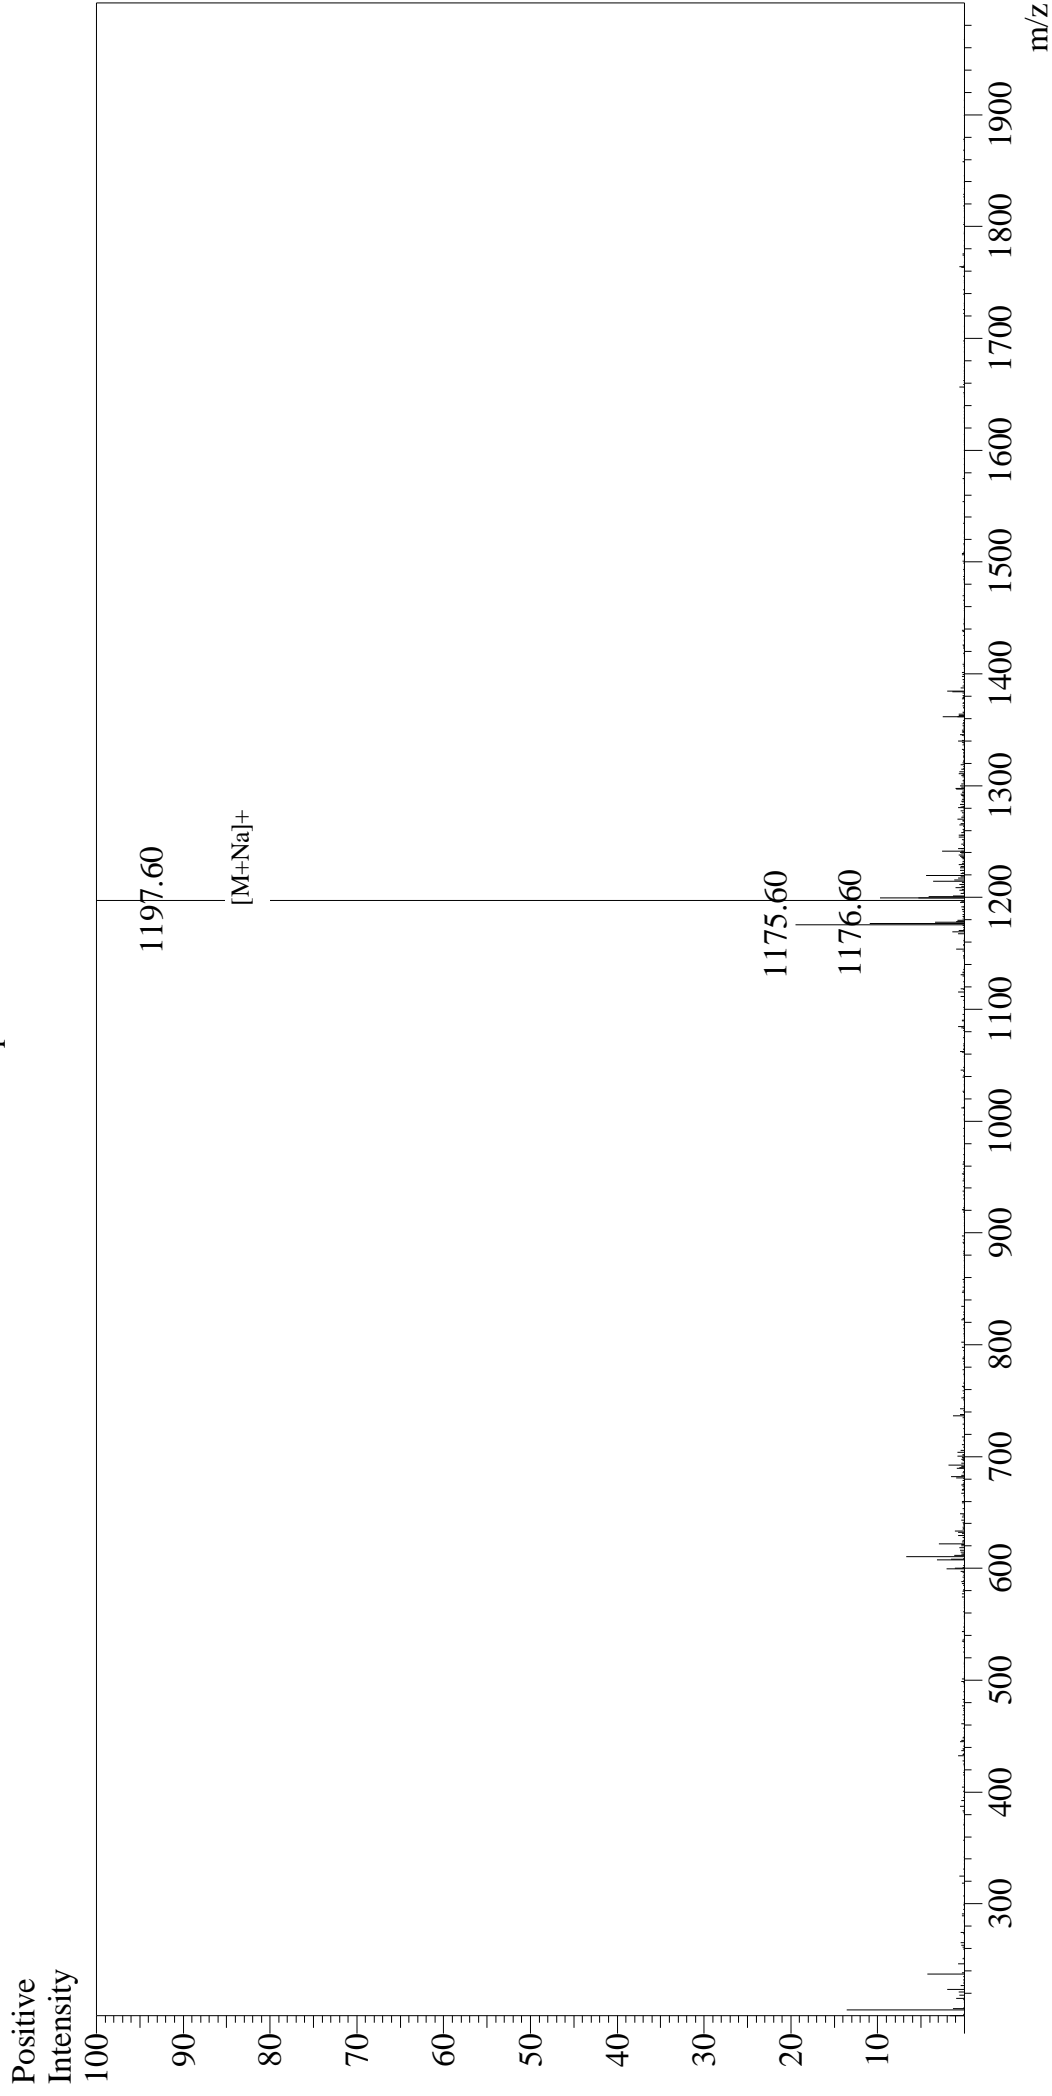

Sample Information

User : Gary
Month-Day Processed : 03/14/17
Time Processed : 11:22:16
Injection Volume : 0.2
Sample Name : mTRP-2(180-188)
Cat No. : RP20250
Lot No. : PE4151703
Theoretical MW : 1175.34
Observed MW : 1175.60

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH