

Sample Name :Influenza A NP(366 - 374) Strain A/PR/8/35
 Cat No. :RP20267
 Lot No. :E5706320C
 Time Processed :8:34:10
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

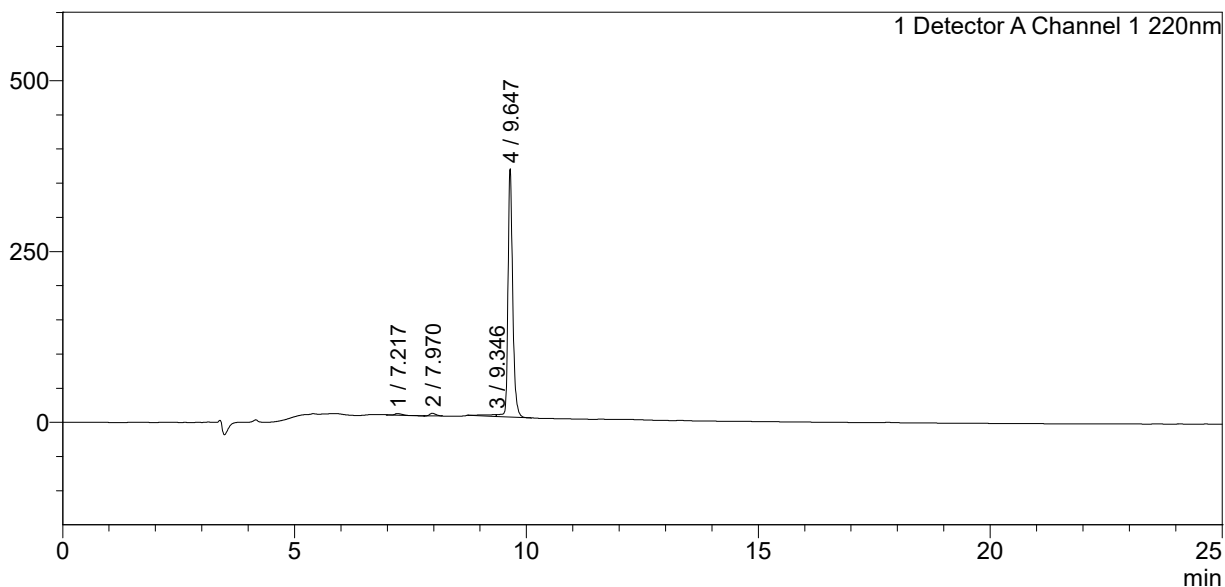

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.217	20996	2348	0.782
2	7.970	34499	3837	1.285
3	9.346	45124	2713	1.681
4	9.647	2583376	363370	96.251
Total		2683995	372267	100.000