


Mass Spectrum

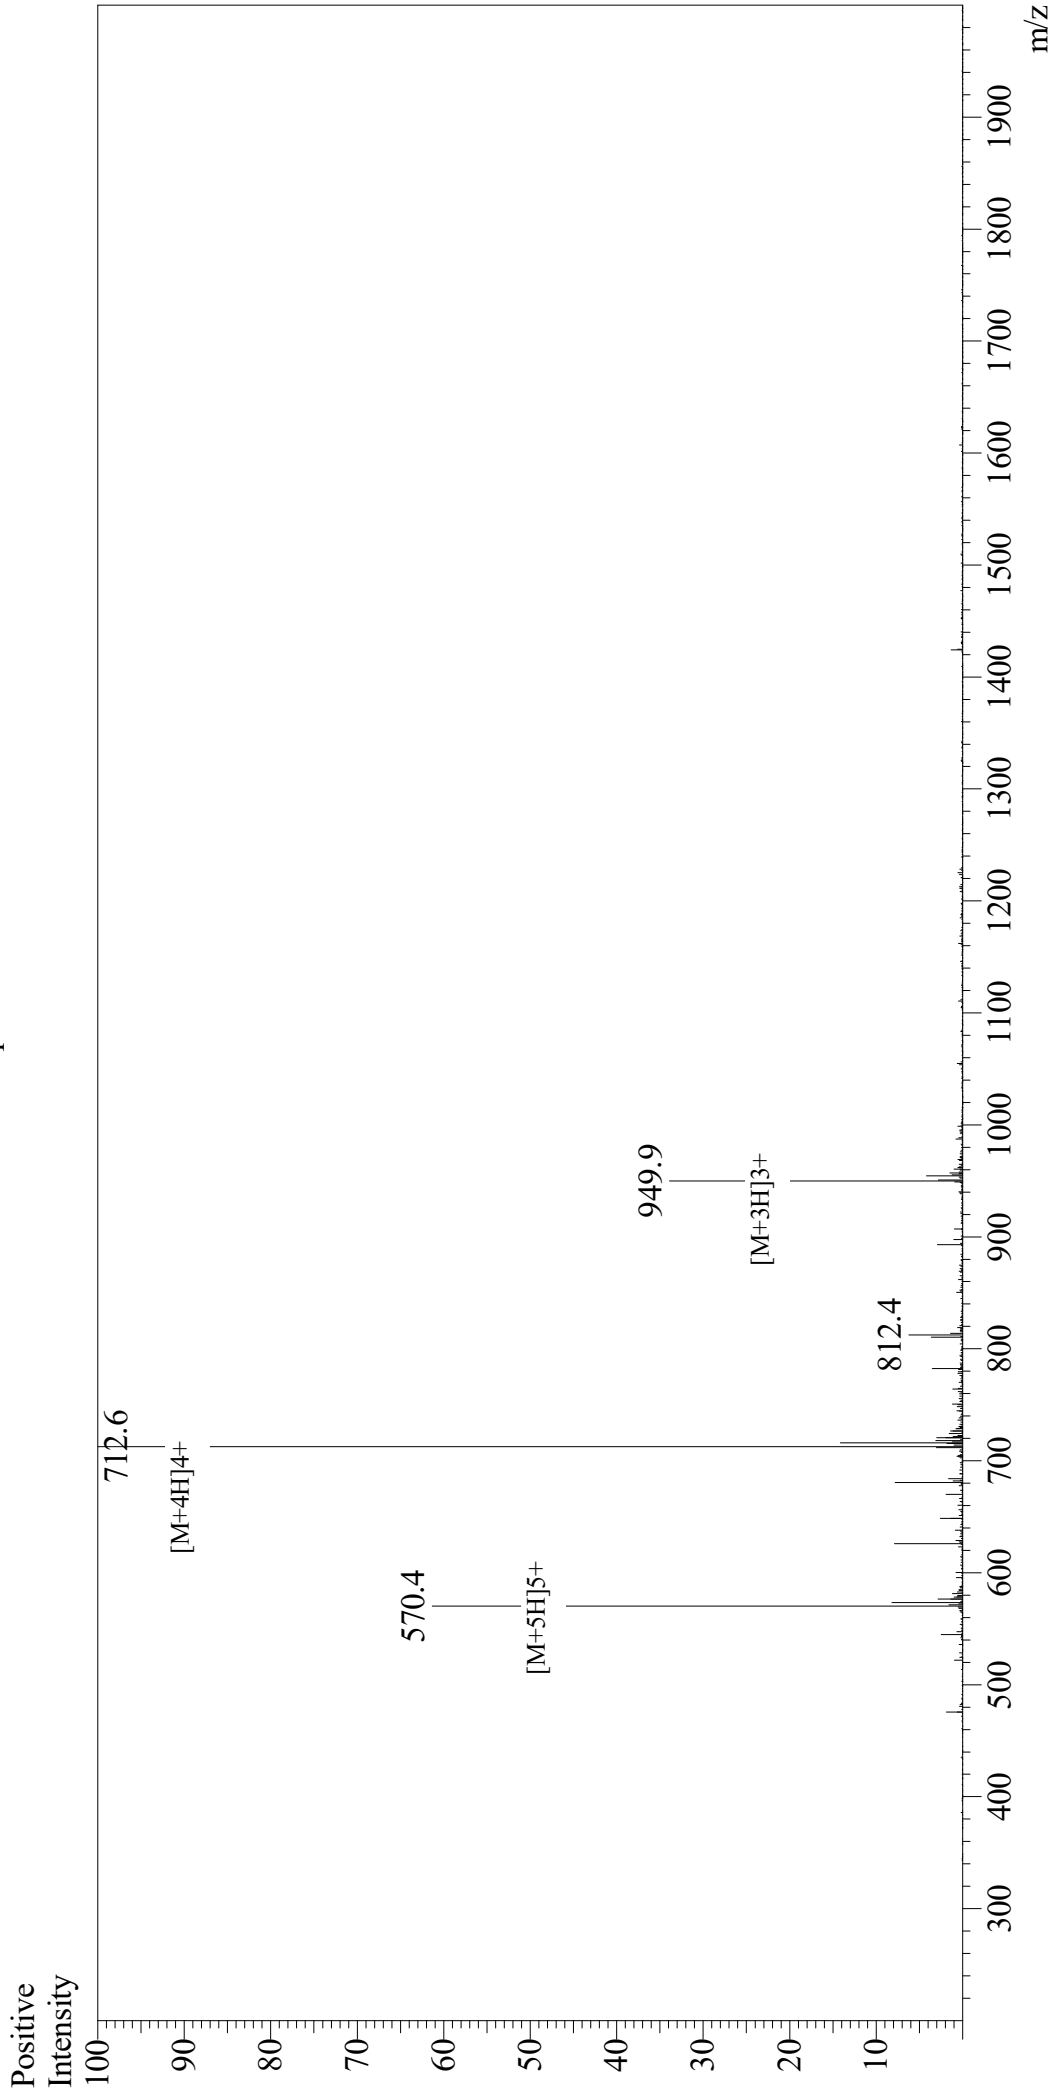

Sample Information

User : Gary
Month-Day Processed : 01/30/19
Time Processed : 09:21:38 AM
Injection Volume : 0.2
Sample Name : Melittin_honey_bee
Cat No. : RP20415
Lot No. : PE2911901
Theoretical MW : 2847.50
Observed MW : 2846.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH