

Sample Name:C-Myc Peptide  
 Cat No :RP11731  
 Lot No :E3607921E  
 Time Processed :4:09:14 PM  
 Month-Day-Year Processed :05/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: SS-CM-0309

### <Chromatogram>

mV

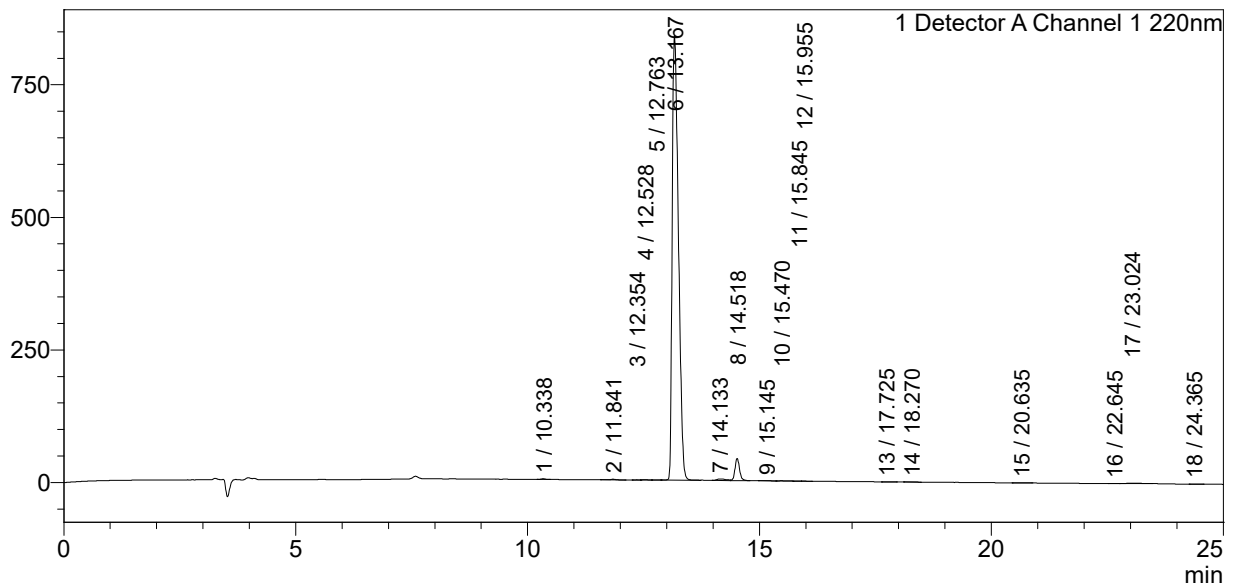

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.338	7373	1216	0.090
2	11.841	11015	1311	0.135
3	12.354	2102	367	0.026
4	12.528	6264	978	0.077
5	12.763	1482	261	0.018
6	13.167	7789557	838337	95.246
7	14.133	39026	2733	0.477
8	14.518	280602	41745	3.431
9	15.145	3216	254	0.039
10	15.470	4634	510	0.057
11	15.845	2091	311	0.026
12	15.955	2214	374	0.027
13	17.725	1727	155	0.021
14	18.270	3312	365	0.040
15	20.635	3242	283	0.040
16	22.645	1085	136	0.013

Peak#	Ret. Time	Area	Height	Area%
17	23.024	18204	829	0.223
18	24.365	1185	173	0.014
Total		8178330	890338	100.000