

Sample Name : Hepatitis B Virus Core (128-140)
 Cat. No. : RP117313
 Lot. No. : E4777020B
 Time Processed : 9:28:33
 Month-Day-Year Processed : 02/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

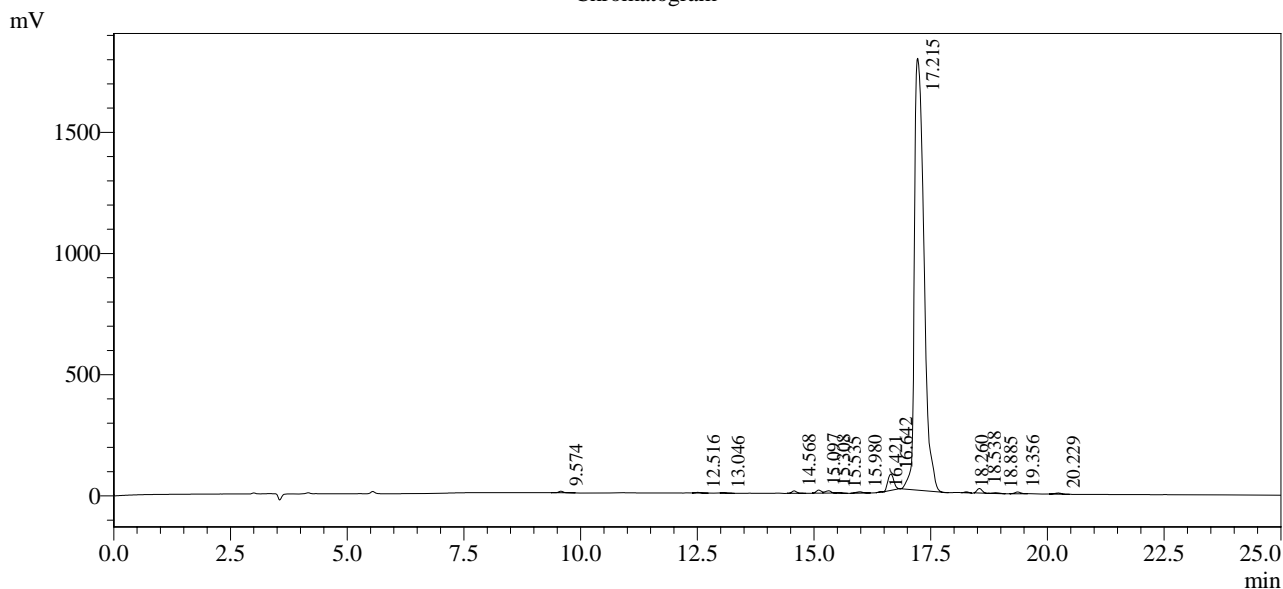

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.574	39530	6201	0.149
2	12.516	17349	2700	0.065
3	13.046	7231	1138	0.027
4	14.568	72954	9891	0.274
5	15.097	96984	12752	0.365
6	15.308	81007	9277	0.305
7	15.535	9789	1362	0.037
8	15.980	64065	5970	0.241
9	16.421	8057	1741	0.030
10	16.642	603255	67078	2.269
11	17.215	25268498	1782257	95.059
12	18.260	24590	3957	0.093
13	18.538	144038	18976	0.542
14	18.885	31781	3246	0.120
15	19.356	64994	7469	0.245
16	20.229	47660	4686	0.179
Total		26581781	1938701	100.000