

Sample Name :Influenza HA (518-526)
 Cat No: RP20284
 Lot. No. :E8547621E
 Time Processed: 11:35:01
 Month-Day-Year Processed :05/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

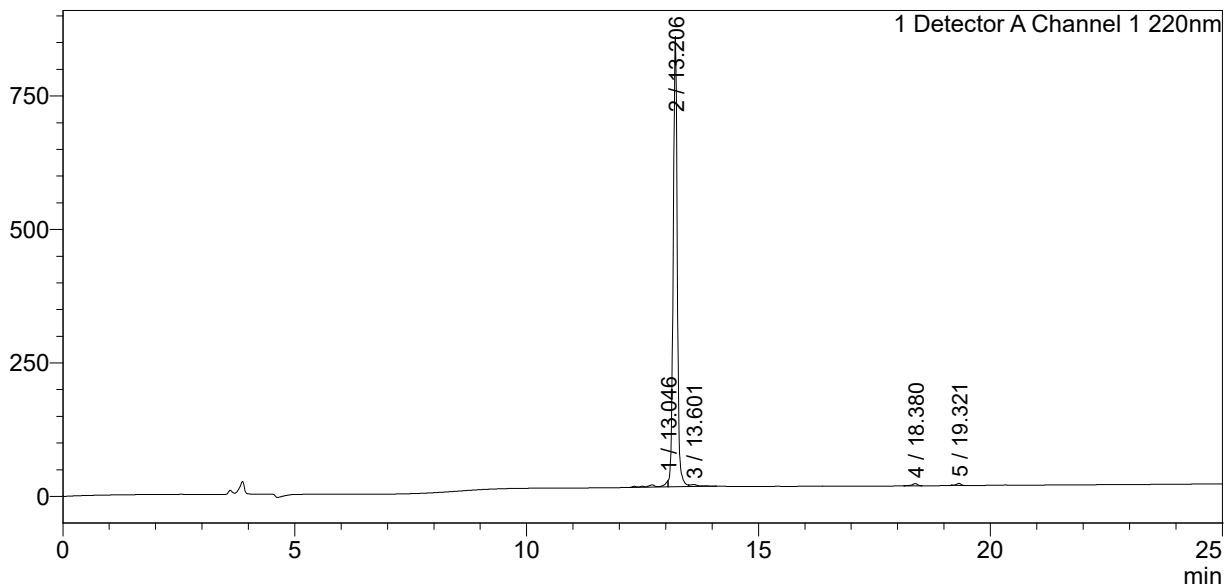

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.046	119598	11036	2.220
2	13.206	5157735	843839	95.735
3	13.601	53037	3890	0.984
4	18.380	32650	4253	0.606
5	19.321	24497	3757	0.455
Total		5387516	866775	100.000