

Sample Name : β -Amyloid (25-35)
 Cat No.: RP10008
 Lot No.: E3430020E
 Time Processed :16:57:51
 Month-Day-Year Processed :06/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
30.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

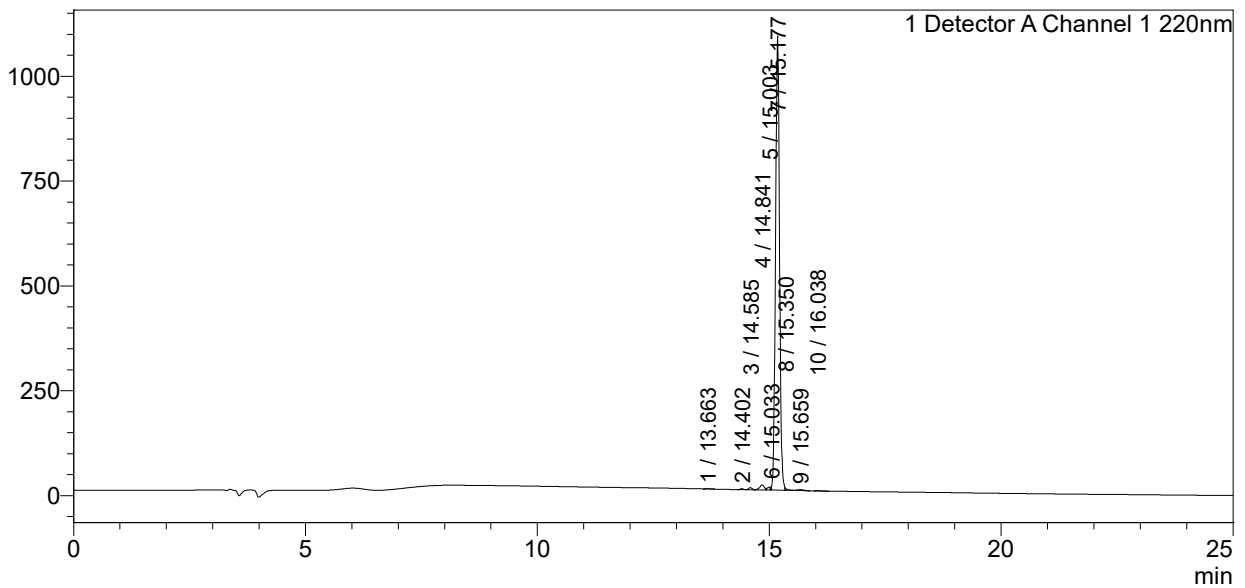

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.663	4272	820	0.064
2	14.402	11784	2338	0.177
3	14.585	28387	5006	0.426
4	14.841	84731	12086	1.270
5	15.003	31006	6709	0.465
6	15.033	6374	6216	0.096
7	15.177	6473751	1083288	97.048
8	15.350	11755	4152	0.176
9	15.659	15518	1920	0.233
10	16.038	3059	492	0.046
Total		6670638	1123027	100.000