

Sample Name :Oxytocin  
 Cat No. : RP10407  
 Lot No. : E4019620H  
 Time Processed : 23:50:52  
 Month-Day-Year Processed : 09/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

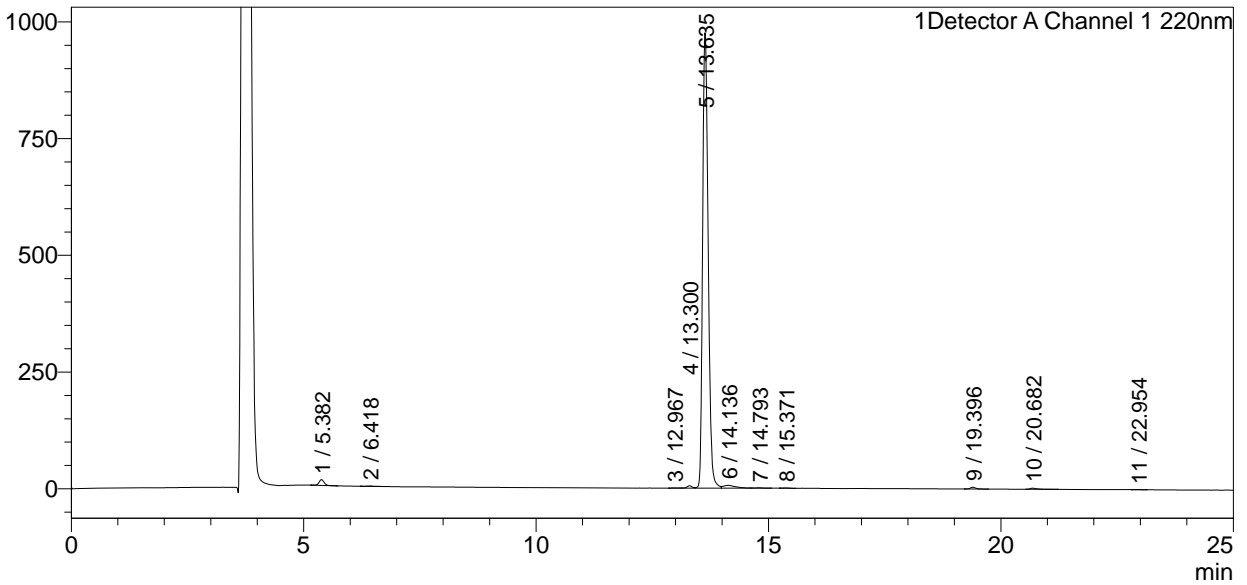

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.382	95191	12412	1.134
2	6.418	6365	896	0.076
3	12.967	3337	269	0.040
4	13.300	38297	4985	0.456
5	13.635	8067626	967420	96.108
6	14.136	111119	6073	1.324
7	14.793	9027	787	0.108
8	15.371	4712	652	0.056
9	19.396	30443	3803	0.363
10	20.682	25174	2275	0.300
11	22.954	3024	355	0.036
Total		8394313	999928	100.000