

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E6774520H
 Time Processed :7:50:09
 Month-Day-Year Processed :08/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

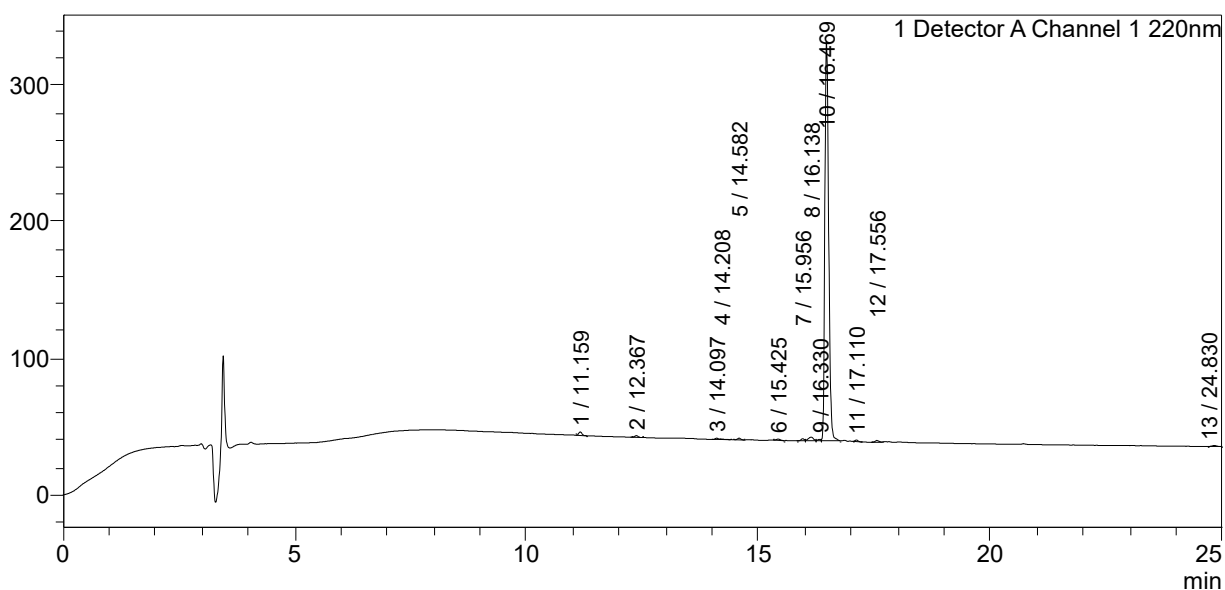

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.159	12075	2607	0.680
2	12.367	6410	1316	0.361
3	14.097	4713	983	0.265
4	14.208	2258	445	0.127
5	14.582	5793	1215	0.326
6	15.425	5366	912	0.302
7	15.956	7898	1547	0.445
8	16.138	19436	2587	1.095
9	16.330	4576	894	0.258
10	16.469	1689202	292757	95.127
11	17.110	5424	1198	0.305
12	17.556	7749	1265	0.436
13	24.830	4833	704	0.272
Total		1775733	308430	100.000