

Sample Name :Mast Cell Degranulating Peptide
 Cat No: RP10663
 Lot No: E4428421A
 Time Processed :20:35:51
 Month-Day-Year Processed :01/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

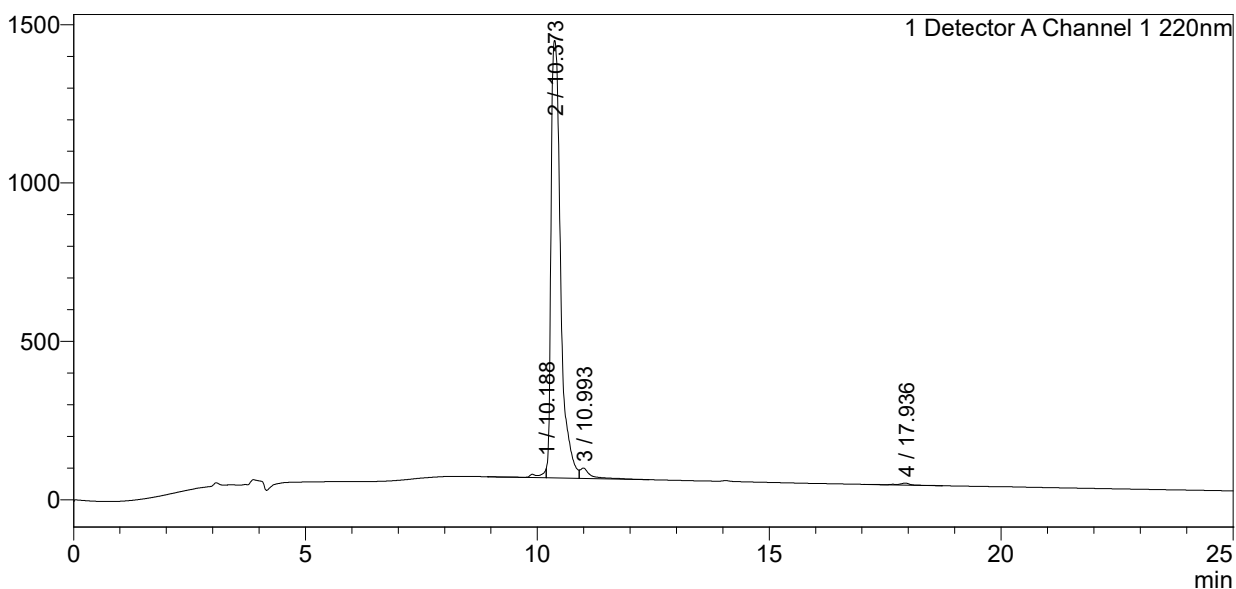

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 10.188 | 244774 | 25239 | 1.187 |
| 2 | 10.373 | 19746036 | 1382153 | 95.720 |
| 3 | 10.993 | 535914 | 33142 | 2.598 |
| 4 | 17.936 | 102179 | 6335 | 0.495 |
| Total | | 20628903 | 1446869 | 100.000 |