

Sample Name :HIV - 1 Rev (34 - 50)  
 Cat No.:RP20362  
 Lot No.: E4957119I  
 Time Processed :8:59:58  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

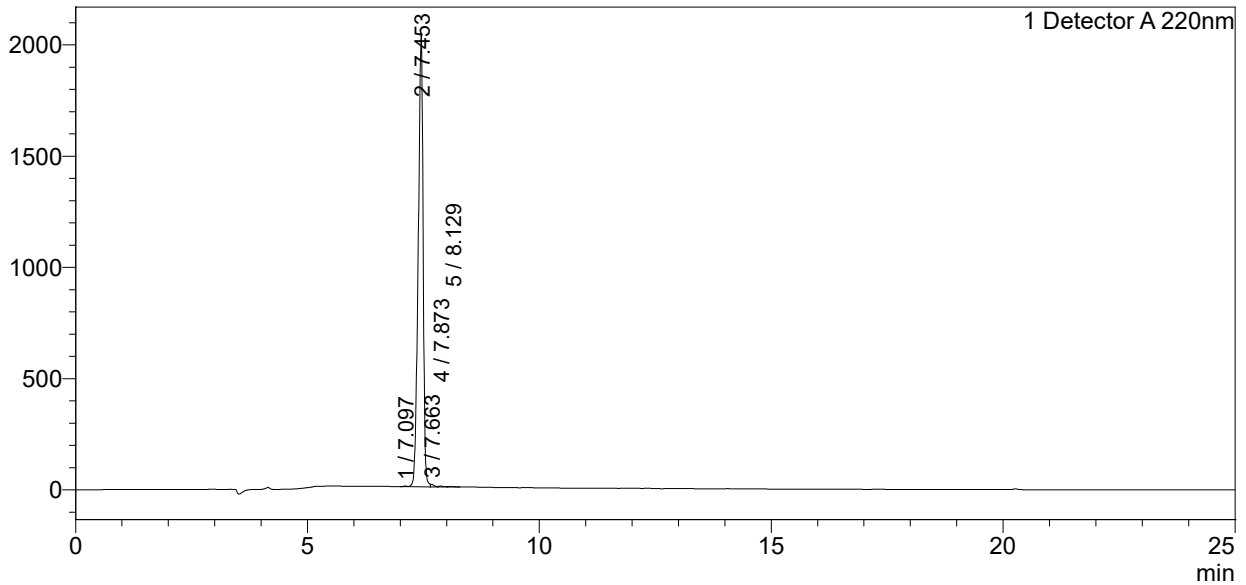

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.097	17111	3057	0.113
2	7.453	14971662	2040482	99.189
3	7.663	59685	11629	0.395
4	7.873	28310	3953	0.188
5	8.129	17285	2399	0.115
Total		15094052	2061519	100.000