


Mass Spectrum

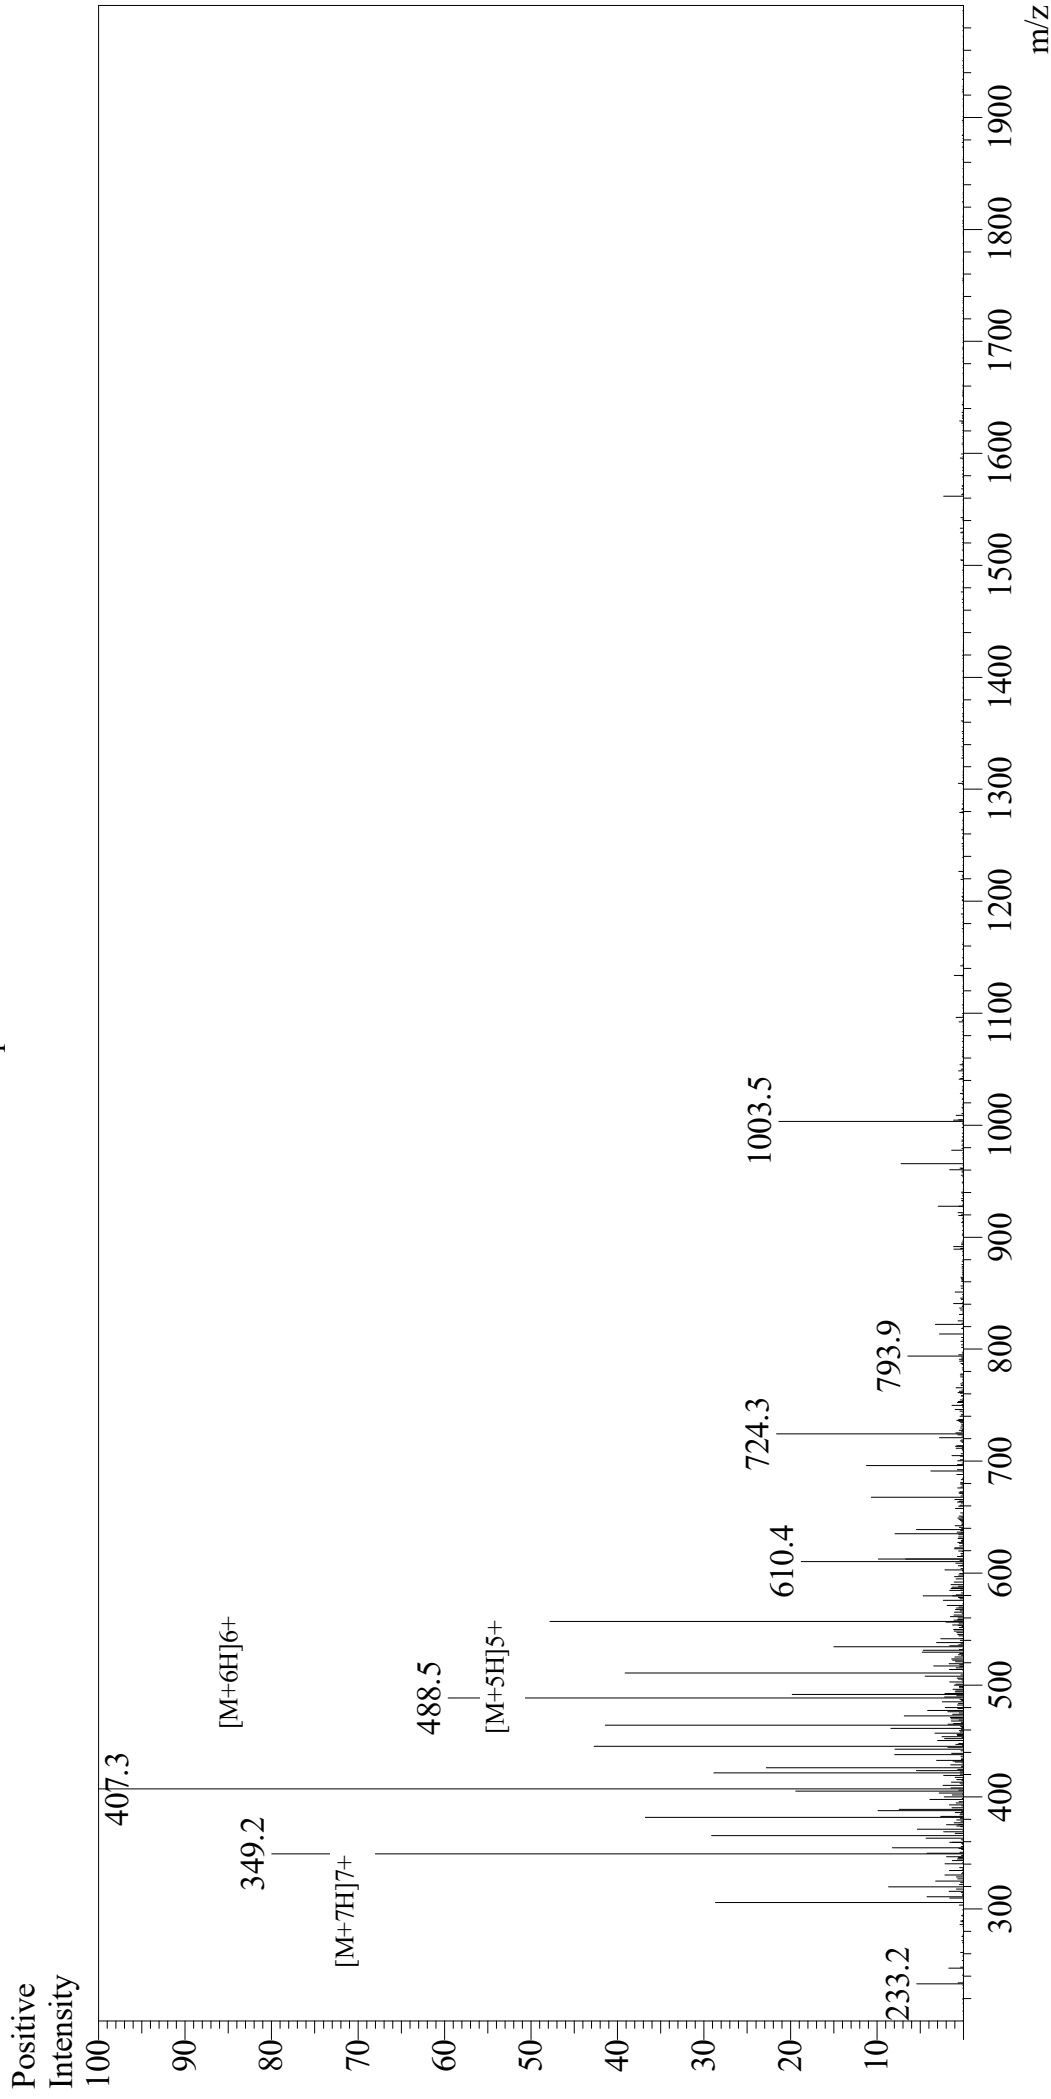

Sample Information

User : Gary
Month-Day Processed : 09/18/19
Time Processed : 02:56:08 PM
Injection Volume : 0.3
Sample Name : HIV - 1 Rev (34 - 50)
Cat No. : RP20362
Lot No. : E4957119I
Theoretical MW : 2437.75
Observed MW : 2437.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH