

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), human, porcine
 Cat. No. : RP11927
 Lot. No. : PE5681903
 Time Processed : 23:17:37
 Month-Day-Year Processed : 03/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
50.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

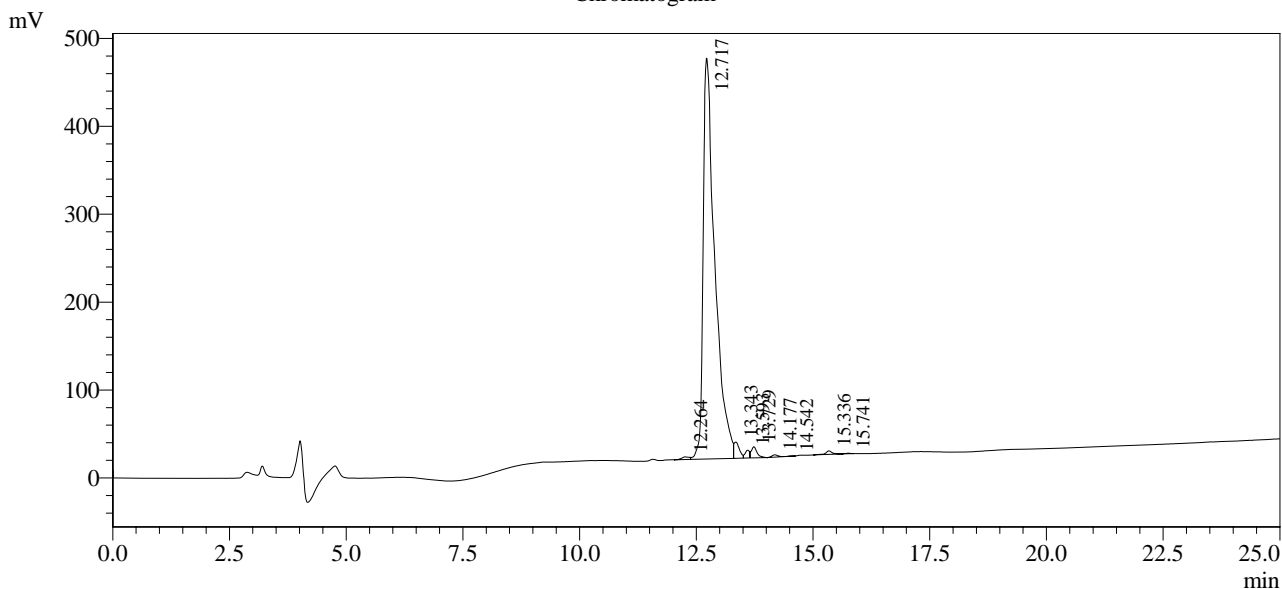

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.264	35317	3154	0.421
2	12.717	7974130	455993	95.039
3	13.343	145534	18505	1.735
4	13.593	59014	8937	0.703
5	13.729	106159	12587	1.265
6	14.177	22787	2569	0.272
7	14.542	1660	200	0.020
8	15.336	40298	4041	0.480
9	15.741	5502	813	0.066
Total		8390399	506800	100.000