

Sample Name :Oxytocin  
 Cat No. :RP10407  
 Lot No. :E8575719H  
 Time Processed :14:26:22  
 Month-Day-Year Processed :09/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

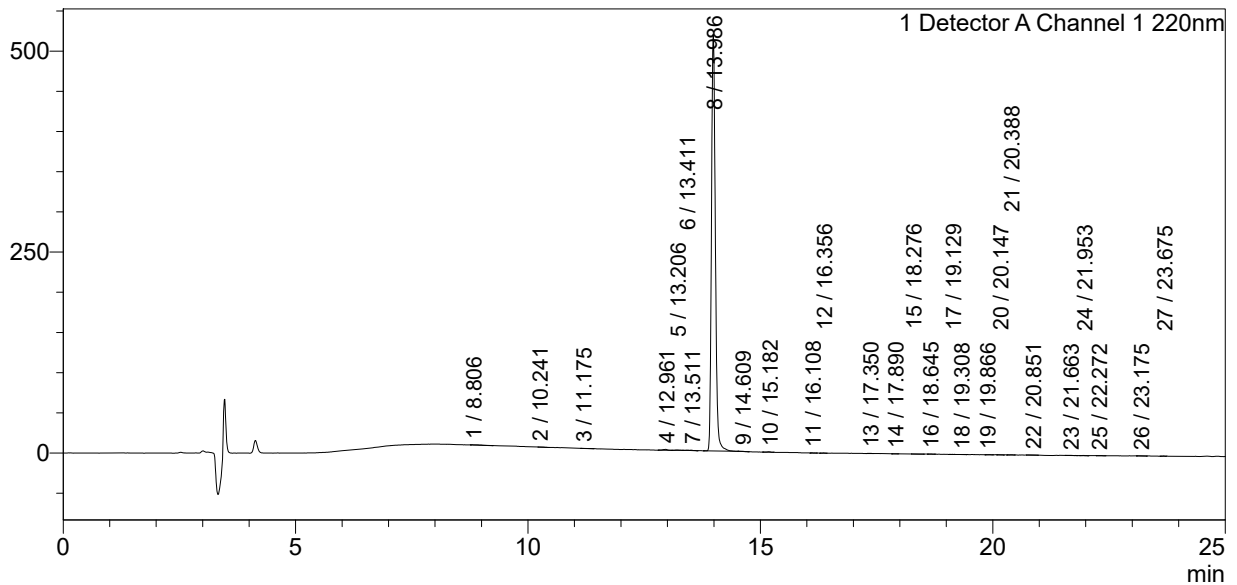

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.806	6426	298	0.209
2	10.241	2332	277	0.076
3	11.175	2387	214	0.078
4	12.961	7035	1027	0.228
5	13.206	3141	486	0.102
6	13.411	2405	368	0.078
7	13.511	2127	482	0.069
8	13.986	3021929	518100	98.143
9	14.609	1628	353	0.053
10	15.182	3356	557	0.109
11	16.108	1069	299	0.035
12	16.356	1233	265	0.040
13	17.350	1923	363	0.062
14	17.890	1024	231	0.033
15	18.276	2050	226	0.067

Peak#	Ret. Time	Area	Height	Area%
16	18.645	1204	260	0.039
17	19.129	1084	130	0.035
18	19.308	1011	188	0.033
19	19.866	1232	187	0.040
20	20.147	1125	224	0.037
21	20.388	1165	203	0.038
22	20.851	4059	495	0.132
23	21.663	1723	202	0.056
24	21.953	1408	257	0.046
25	22.272	1424	194	0.046
26	23.175	2571	381	0.084
27	23.675	1035	280	0.034
Total		3079105	526548	100.000