

Sample Name :GroES mobile loop
 Cat No. :RP20179
 Lot No. :E5570319J
 Time Processed :8:01:44 PM
 Month-Day-Year Processed :10/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

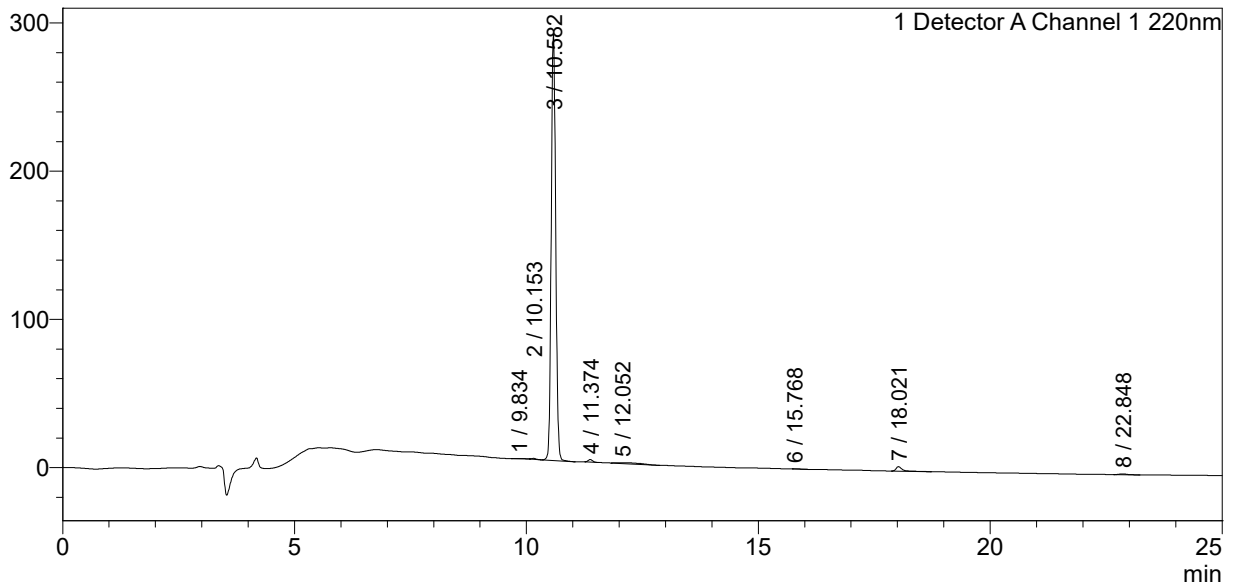

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.834	2964	210	0.147
2	10.153	3561	601	0.176
3	10.582	1940382	287697	96.093
4	11.374	11492	1751	0.569
5	12.052	24123	530	1.195
6	15.768	1019	47	0.050
7	18.021	29159	3012	1.444
8	22.848	6570	540	0.325
Total		2019271	294388	100.000