

Sample Name :Flu-M1 (58-66)

Cat. No. : RP19978

Lot. No. : PE2561811

Time Processed :9:44:58

Month-Day-Year Processed :11/02/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 5 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.01 | Pumps | Pump A B.Conc | 95 | |
| 27.00 | Pumps | Pump A B.Conc | 95 | |
| 27.01 | Pumps | Pump A B.Conc | 5 | |
| 35.00 | Pumps | Pump A B.Conc | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:GK11010009

Chromatogram

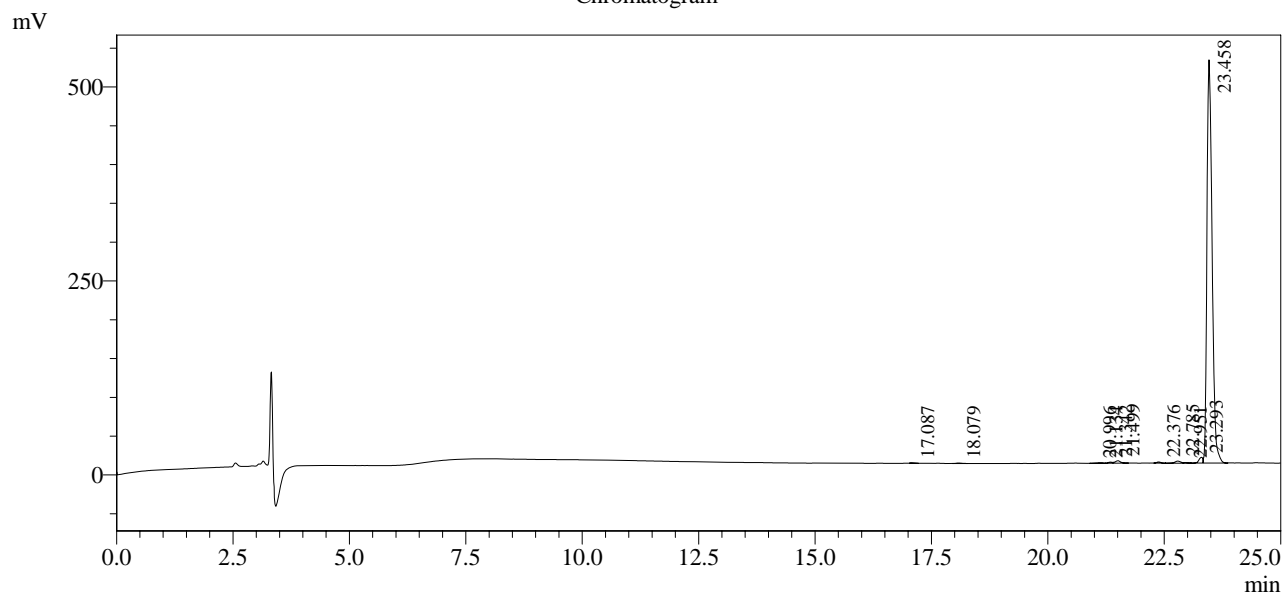

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 17.087 | 2352 | 453 | 0.057 |
| 2 | 18.079 | 4806 | 645 | 0.116 |
| 3 | 20.996 | 1385 | 290 | 0.033 |
| 4 | 21.134 | 3662 | 522 | 0.088 |
| 5 | 21.342 | 8419 | 1328 | 0.203 |
| 6 | 21.499 | 23063 | 2973 | 0.556 |
| 7 | 22.376 | 9481 | 1629 | 0.229 |
| 8 | 22.785 | 23212 | 2603 | 0.560 |
| 9 | 22.951 | 3630 | 682 | 0.088 |
| 10 | 23.293 | 43696 | 7389 | 1.054 |
| 11 | 23.458 | 4022214 | 519496 | 97.016 |
| Total | | 4145919 | 538011 | 100.000 |