

Sample Name : LL37 (Human)  
 Cat. No. : RP13323  
 Lot. No. : E4084221G  
 Time Processed :1:04:01 AM  
 Month-Day-Year Processed :07/17/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

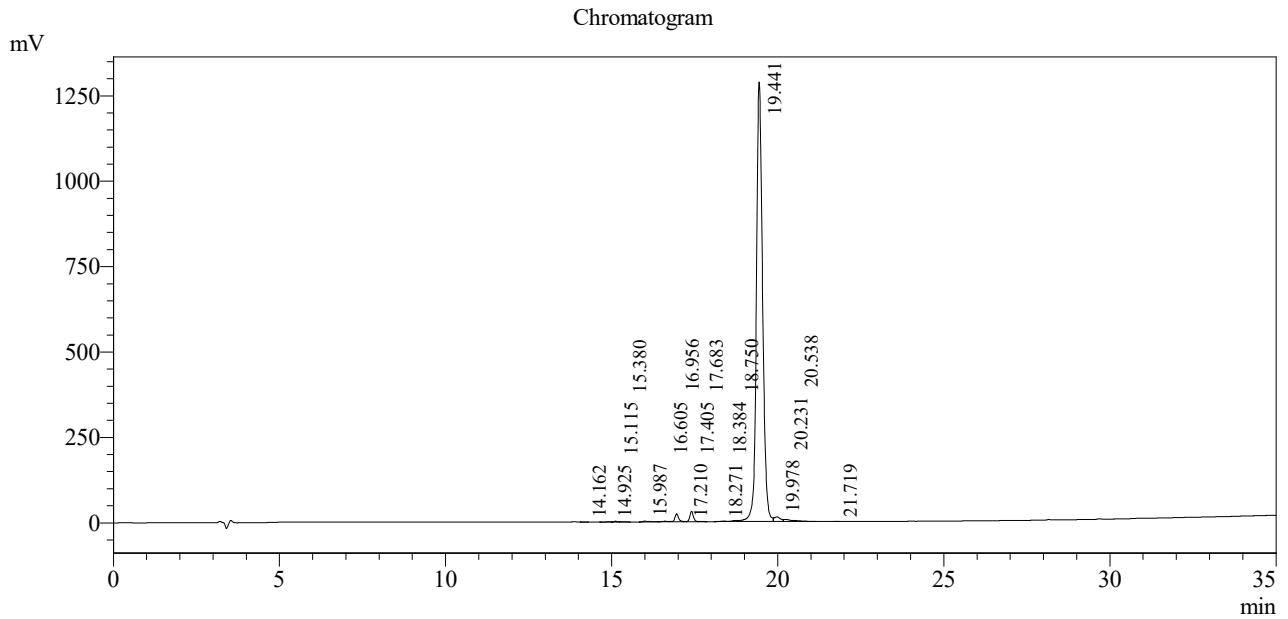

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.162	450	65	0.003
2	14.925	5286	397	0.030
3	15.115	14718	2206	0.084
4	15.380	7471	776	0.043
5	15.987	32737	2187	0.187
6	16.605	18552	1774	0.106
7	16.956	181678	23147	1.040
8	17.210	7635	1329	0.044
9	17.405	223035	30208	1.276
10	17.683	8501	1051	0.049
11	18.271	2626	477	0.015
12	18.384	13258	1304	0.076
13	18.750	38657	3181	0.221
14	19.441	16612561	1286816	95.075
15	19.978	178745	13437	1.023
16	20.231	93434	6036	0.535
17	20.538	33711	2493	0.193
18	21.719	61	10	0.000
Total		17473115	1376894	100.000