

Sample Name : [Glu1]-Fibrinopeptide B
 Cat No: RP20439
 Lot No : E0180321D
 Time Processed : 13:58:30
 Month-Day-Year Processed : 04/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

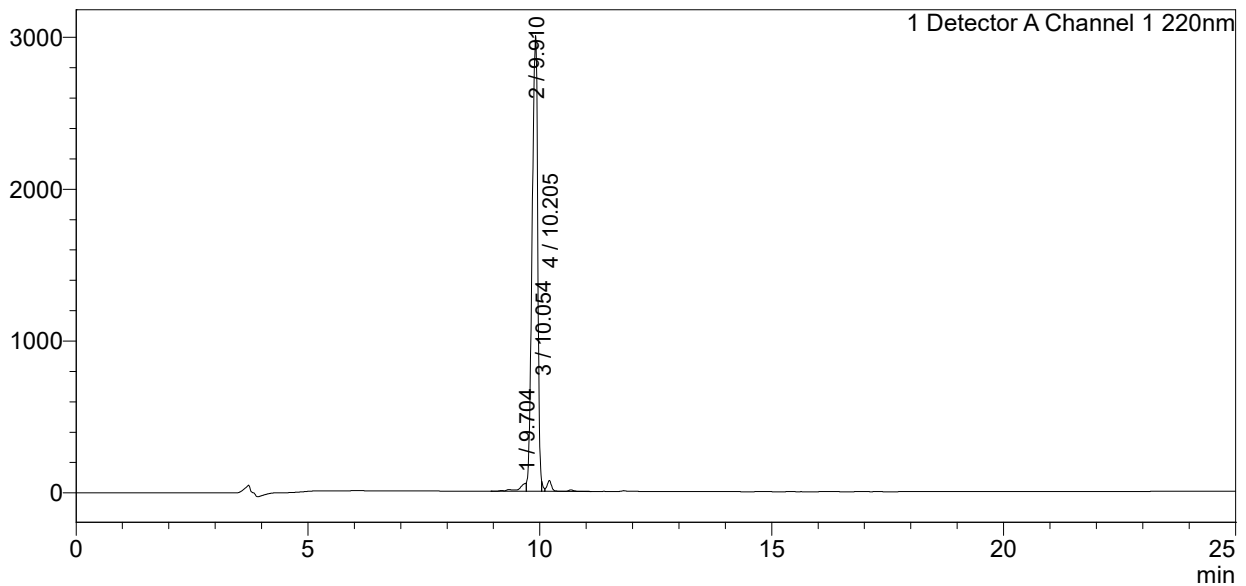

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.704	588175	53276	2.202
2	9.910	25432762	3001909	95.229
3	10.054	118646	52564	0.444
4	10.205	567240	71705	2.124
Total		26706822	3179455	100.000