

Sample Name : Peptide C105Y
 Cat No. : RP20382
 Lot No. : E5610520E
 Time Processed: 15:16:13
 Month-Day-Year Processed :05/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010324

<Chromatogram>

mV

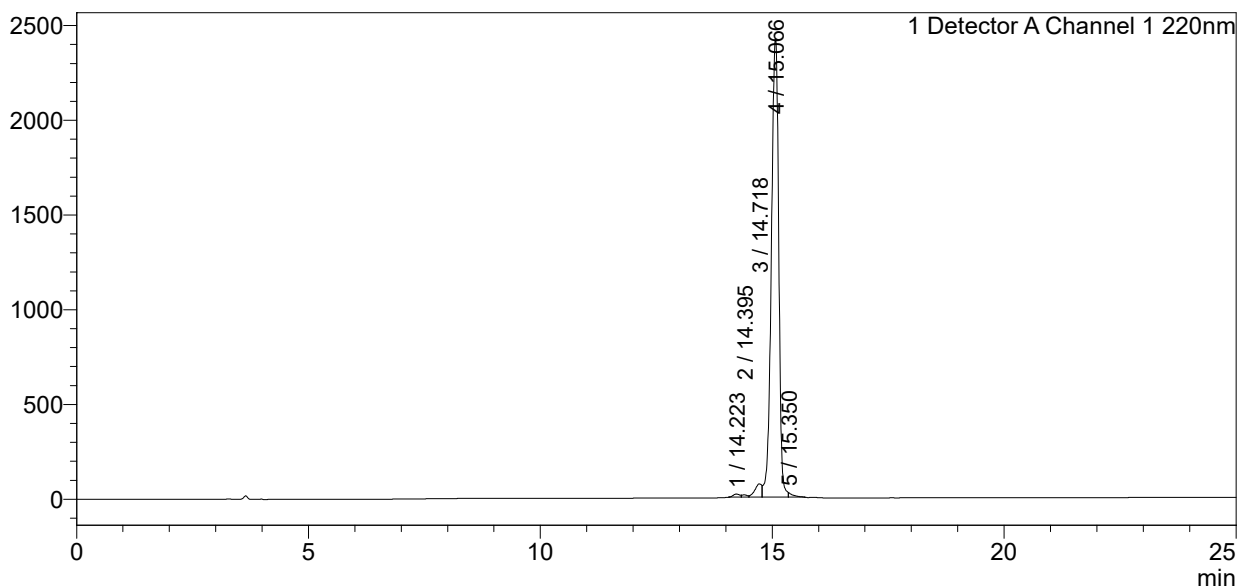

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.223	168135	16796	0.604
2	14.395	103371	12562	0.371
3	14.718	733949	70435	2.635
4	15.066	26688858	2421016	95.805
5	15.350	163030	24561	0.585
Total		27857342	2545370	100.000