


Mass Spectrum

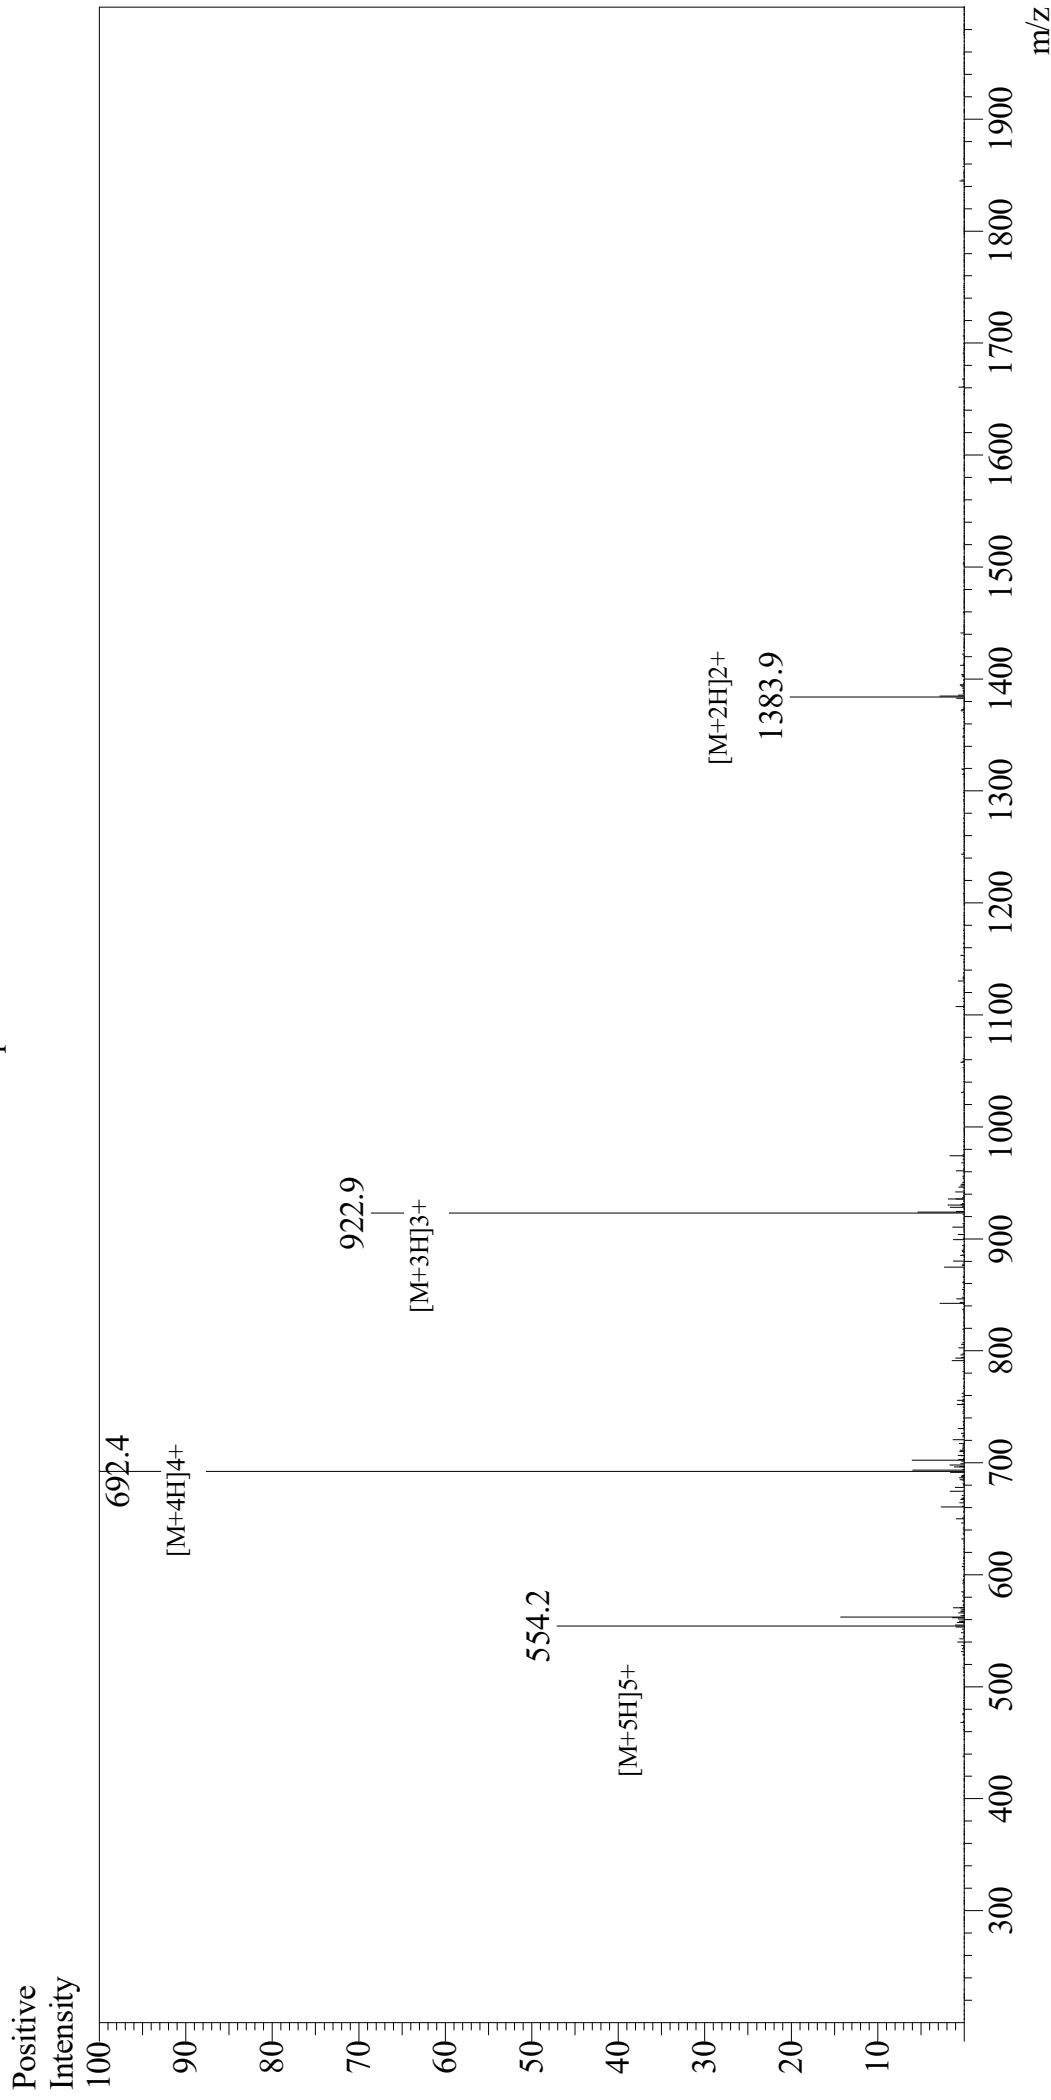

Sample Information

User : Gary
Month-Day Processed : 10/02/19
Time Processed : 06:40:11 PM
Injection Volume : 0.3
Sample Name : MPG, HIV related
Cat No. : RP20335
Lot No. : E7067019J
Theoretical MW : 2766.20
Observed MW : 2765.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH