

Sample Name : β -Endorphin, human
 Cat No.: RP11344
 Lot No.: E7545220B
 Time Processed :19:02:34
 Month-Day-Year Processed :02/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

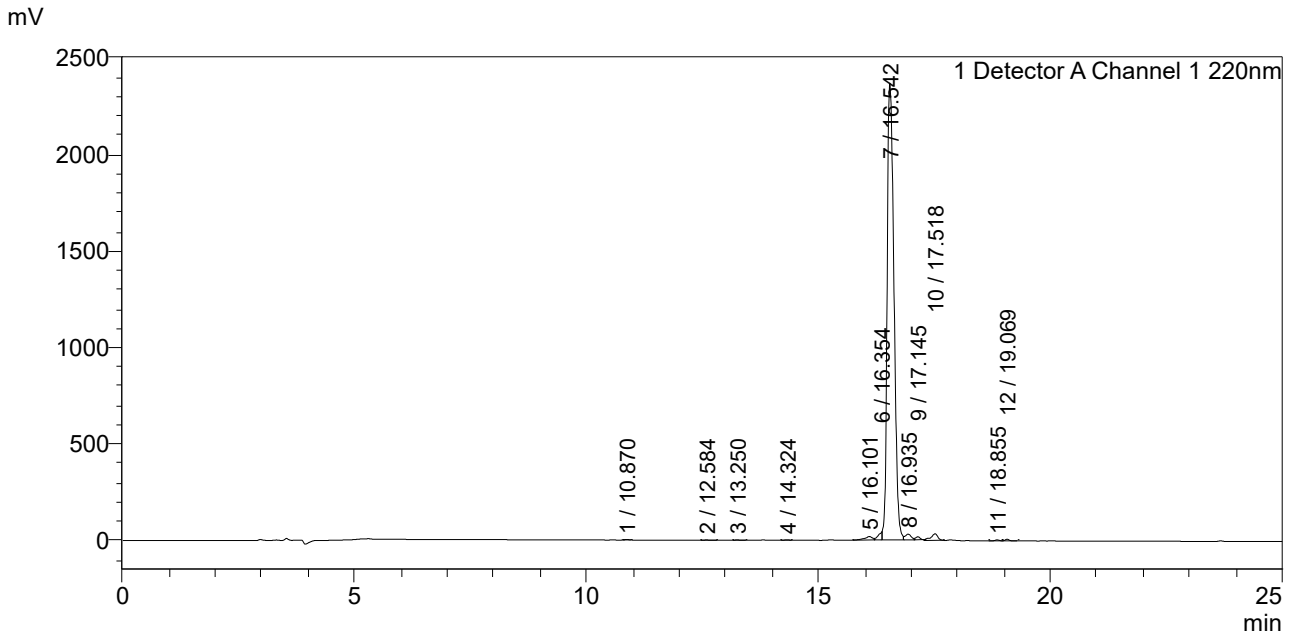

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.870	14216	2557	0.056
2	12.584	6867	1060	0.027
3	13.250	12711	2133	0.050
4	14.324	12406	2205	0.049
5	16.101	210739	17983	0.835
6	16.354	194849	34996	0.772
7	16.542	23998959	2368047	95.082
8	16.935	251443	28864	0.996
9	17.145	99316	15164	0.393
10	17.518	355163	33895	1.407
11	18.855	32451	5336	0.129
12	19.069	51216	8698	0.203
Total		25240336	2520938	100.000