

Sample Name :GP (33-41)
 Cat. No. : RP20091
 Lot. No. : PE8781902
 Time Processed : 11:00:33
 Month-Day-Year Processed : 03/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
32.00	Pumps	Pump B Conc.	95	
32.01	Pumps	Pump B Conc.	15	
40.00	Pumps	Pump B Conc.	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

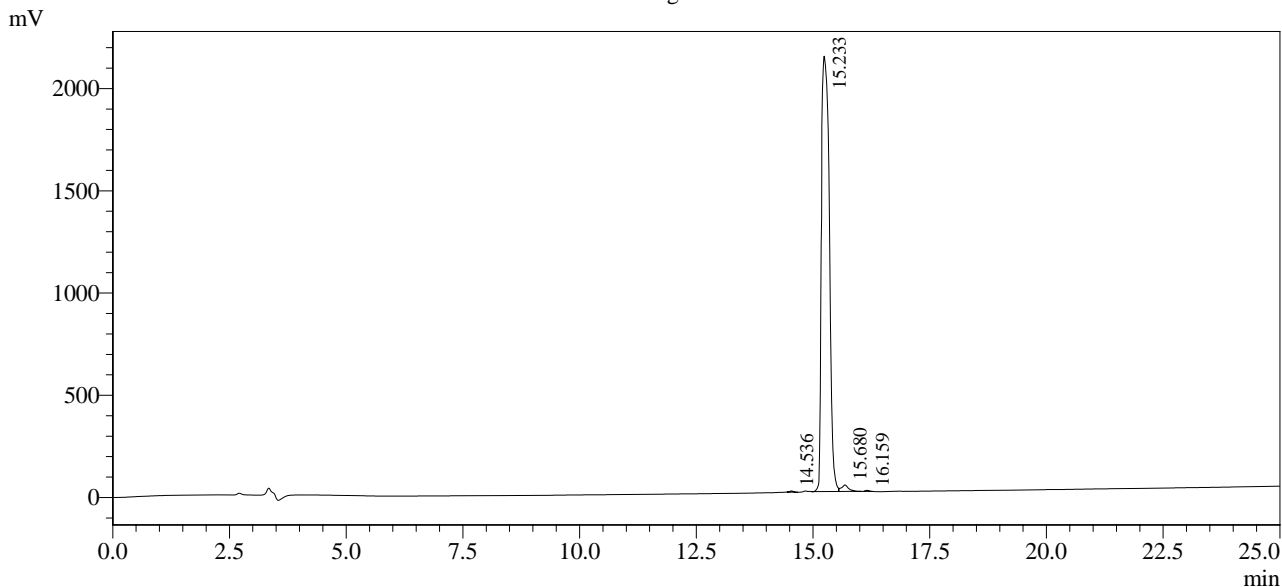

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.536	31115	6119	0.123
2	15.233	24984597	2128947	98.455
3	15.680	334555	31499	1.318
4	16.159	26462	5355	0.104
Total		25376729	2171919	100.000