


Mass Spectrum

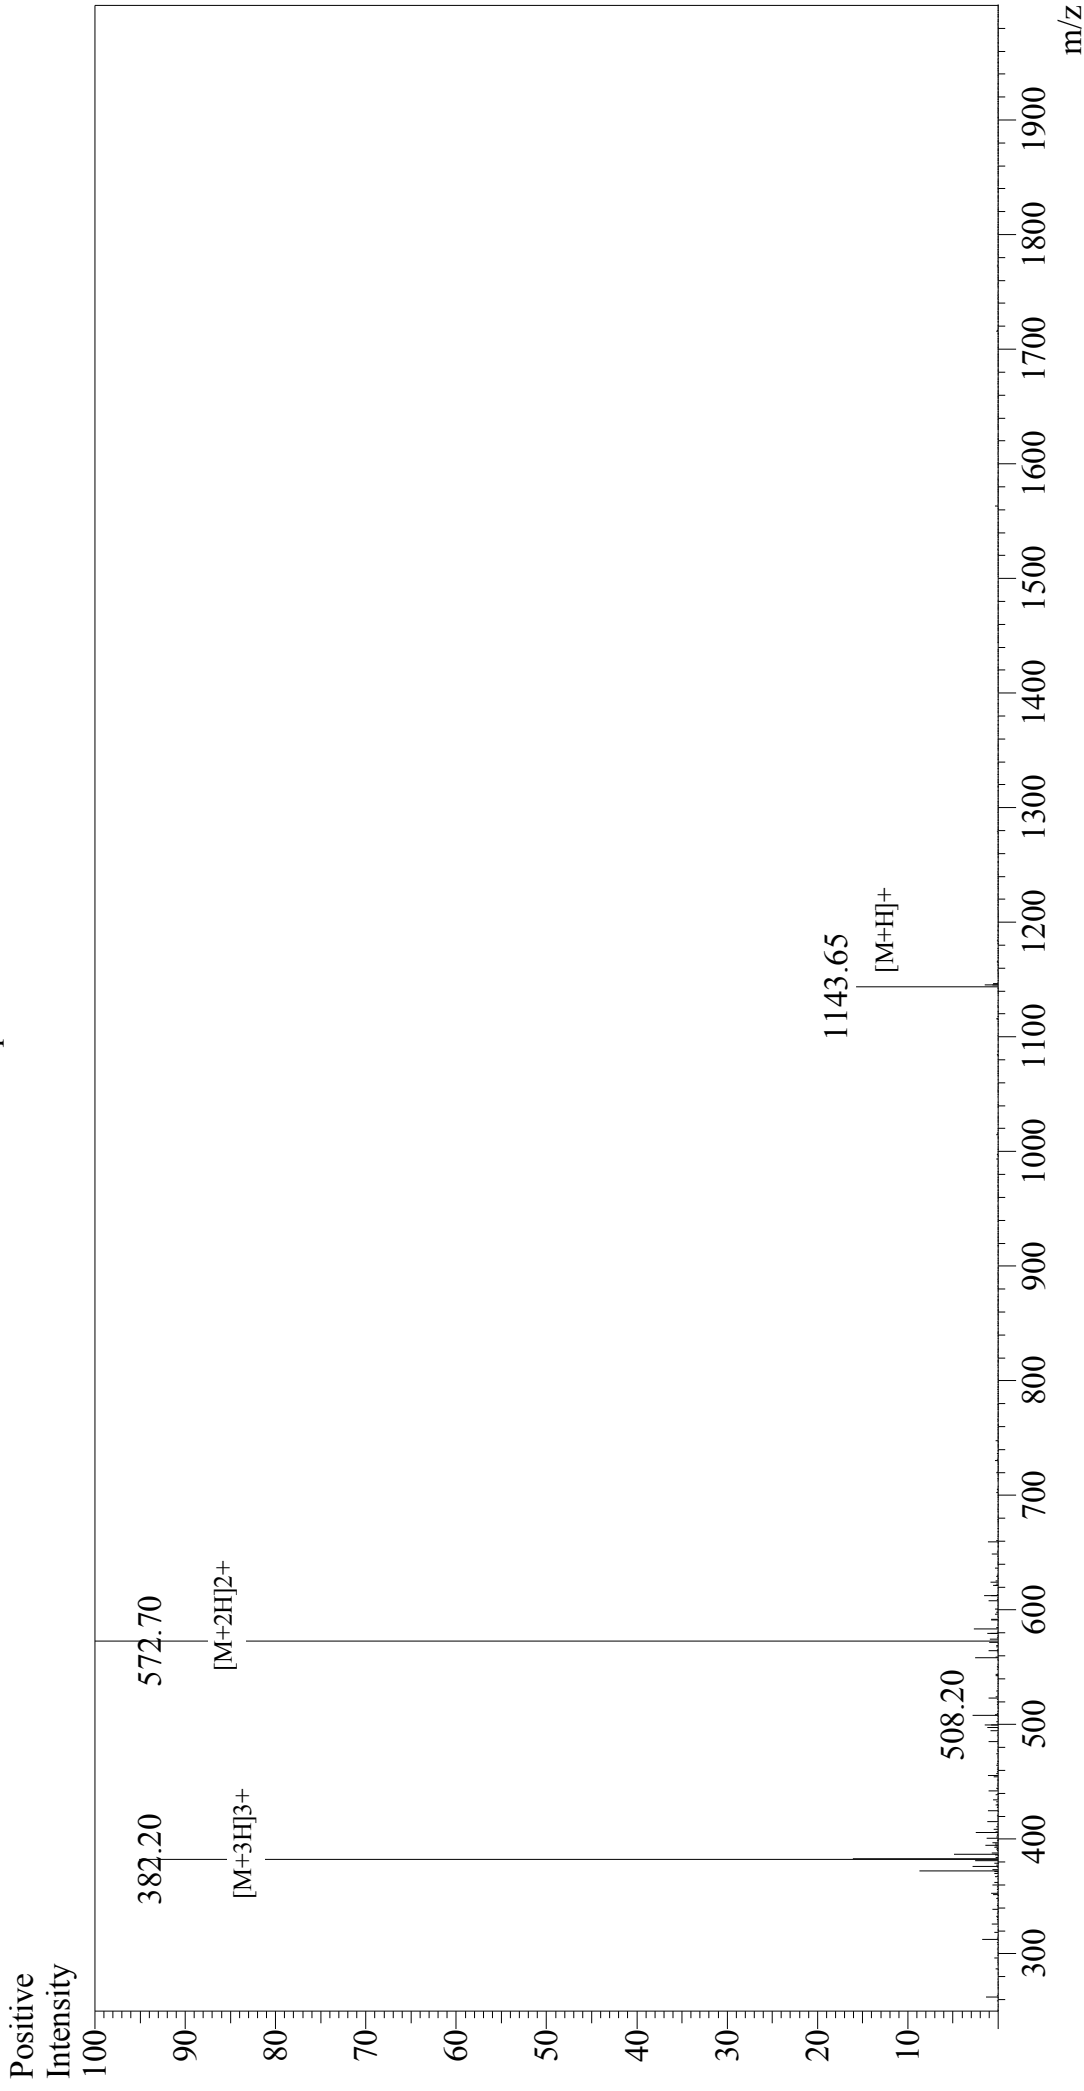

Sample Information

Acquired by : Gary
Month-Day Processed : 09/30/17
Time Processed : 10:41:13
Injection Volume : 0.2
Sample Name : CEF27_EBV BRLF-1 lytic (148 - 156)
Cat.No: RP20397
Lot.No: PE8941709
Theoretical MW : 1143.30
Observed MW : 1143.40

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH