

Sample Name :Influenza HA (518-526)
 Cat No: RP20284
 Lot No : E9428821D
 Time Processed :16:25:28
 Month-Day-Year Processed :04/29/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

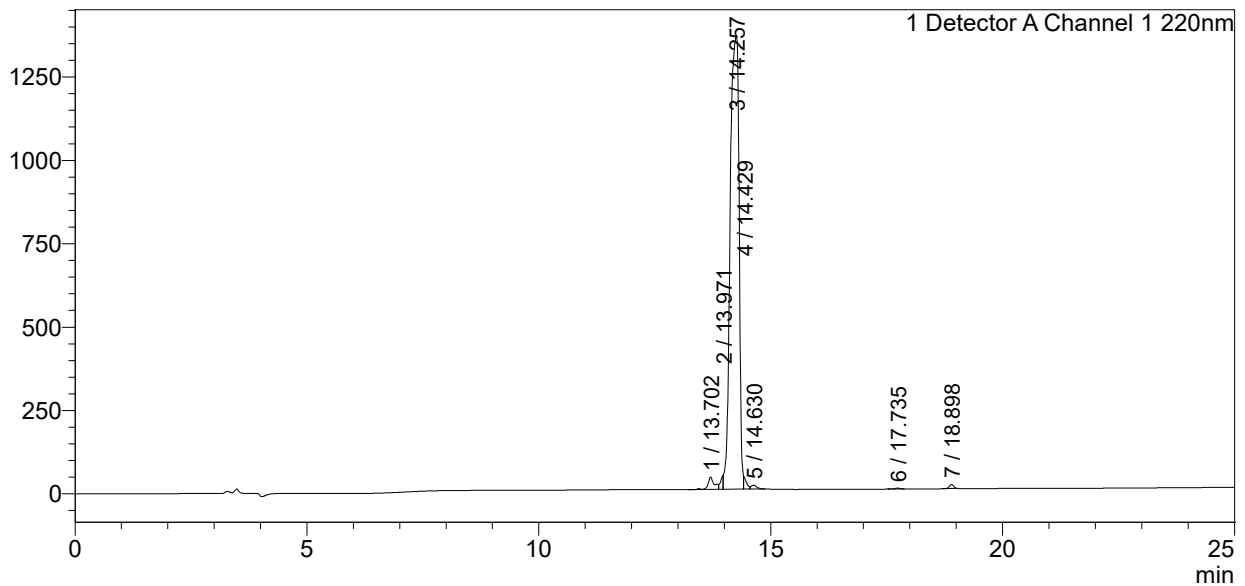

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 13.702 | 343530 | 37064 | 1.821 |
| 2 | 13.971 | 164458 | 40096 | 0.872 |
| 3 | 14.257 | 18008113 | 1360276 | 95.475 |
| 4 | 14.429 | 150565 | 36957 | 0.798 |
| 5 | 14.630 | 99325 | 11454 | 0.527 |
| 6 | 17.735 | 18196 | 2474 | 0.096 |
| 7 | 18.898 | 77393 | 12120 | 0.410 |
| Total | | 18861579 | 1500441 | 100.000 |