

Sample Name :Osteogenic Growth Peptide, OGP
 Cat. No. : RP20311
 Lot. No. : E7291819H
 Time Processed : 22:45:40
 Month-Day-Year Processed :08/30/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:SS-CM-0286

Chromatogram

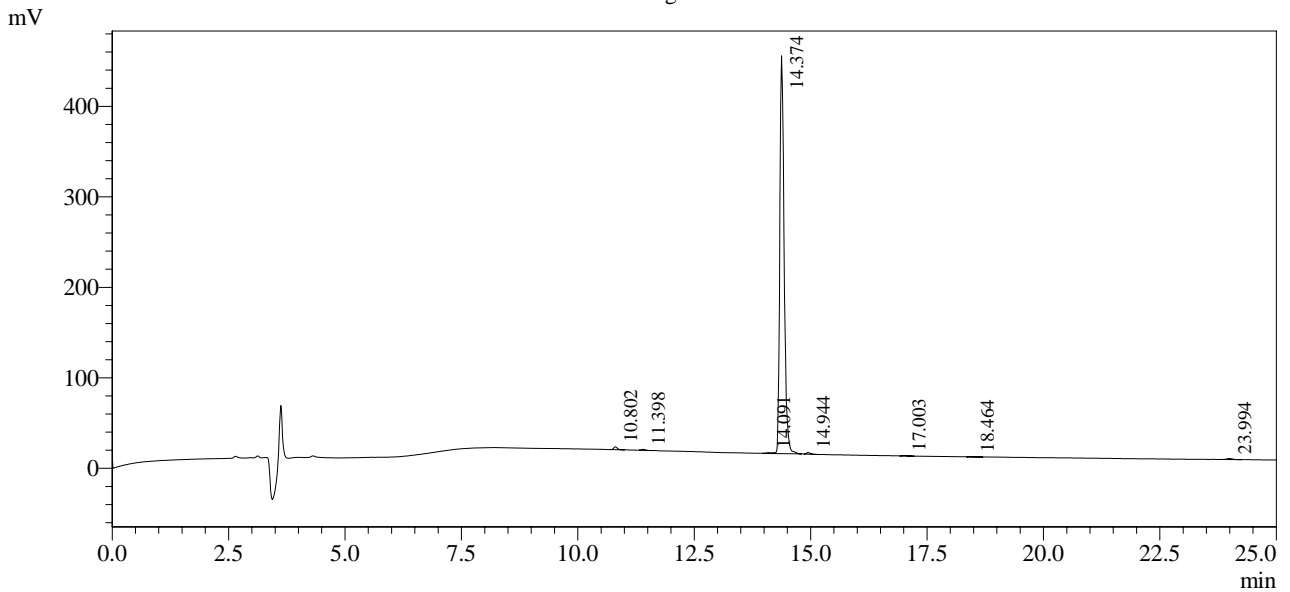

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.802	17063	3177	0.587
2	11.398	5487	1056	0.189
3	14.091	6841	866	0.235
4	14.374	2853935	439496	98.122
5	14.944	9822	1751	0.338
6	17.003	2168	344	0.075
7	18.464	2763	321	0.095
8	23.994	10475	1187	0.360
Total		2908554	448199	100.000