

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. : RP11529
 Lot No. : E1324921F
 Time Processed : 4:11:40
 Month-Day-Year Processed : 06/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 10.00 | Pumps | Pump B Conc. | 35 |
| 35.00 | Pumps | Pump B Conc. | 95 |
| 37.00 | Pumps | Pump B Conc. | 95 |
| 37.01 | Pumps | Pump B Conc. | 5 |
| 42.00 | Pumps | Pump B Conc. | 5 |
| 42.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

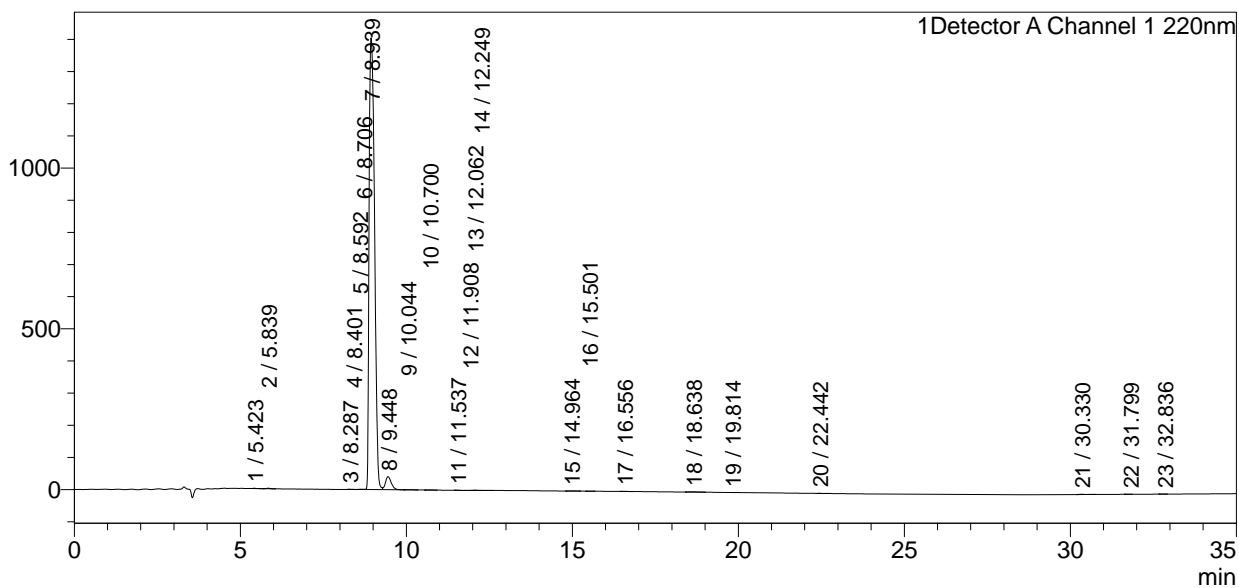

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|--------|
| 1 | 5.423 | 7447 | 1047 | 0.045 |
| 2 | 5.839 | 12324 | 1844 | 0.075 |
| 3 | 8.287 | 4580 | 836 | 0.028 |
| 4 | 8.401 | 1570 | 327 | 0.009 |
| 5 | 8.592 | 2164 | 440 | 0.013 |
| 6 | 8.706 | 4529 | 708 | 0.027 |
| 7 | 8.939 | 15945460 | 1405104 | 96.452 |
| 8 | 9.448 | 494931 | 40427 | 2.994 |
| 9 | 10.044 | 3761 | 305 | 0.023 |
| 10 | 10.700 | 4365 | 378 | 0.026 |
| 11 | 11.537 | 2991 | 513 | 0.018 |
| 12 | 11.908 | 1072 | 162 | 0.006 |
| 13 | 12.062 | 6937 | 776 | 0.042 |
| 14 | 12.249 | 2604 | 219 | 0.016 |
| 15 | 14.964 | 4491 | 442 | 0.027 |

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 16 | 15.501 | 1689 | 235 | 0.010 |
| 17 | 16.556 | 2301 | 247 | 0.014 |
| 18 | 18.638 | 10567 | 581 | 0.064 |
| 19 | 19.814 | 1710 | 228 | 0.010 |
| 20 | 22.442 | 2389 | 270 | 0.014 |
| 21 | 30.330 | 10492 | 930 | 0.063 |
| 22 | 31.799 | 1173 | 144 | 0.007 |
| 23 | 32.836 | 2466 | 339 | 0.015 |
| Total | | 16532013 | 1456503 | 100.000 |