

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : E6967821K
 Time Processed : 22:12:39
 Month-Day-Year Processed : 11/15/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 5 |
| 35.00 | Pumps | B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

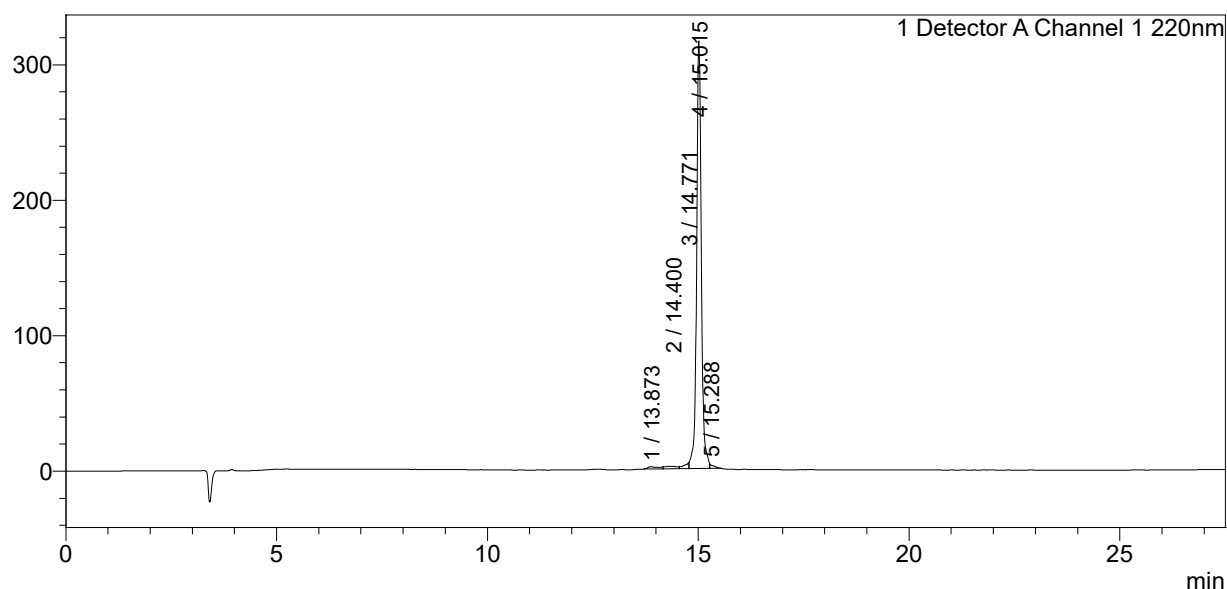

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 13.873 | 29438 | 1601 | 1.145 |
| 2 | 14.400 | 36208 | 1675 | 1.408 |
| 3 | 14.771 | 33240 | 4120 | 1.293 |
| 4 | 15.015 | 2452611 | 315819 | 95.377 |
| 5 | 15.288 | 20004 | 3015 | 0.778 |
| Total | | 2571501 | 326230 | 100.000 |