

Sample Name: Men 10376
 Cat No. : RP10468
 Lot No. : E6994619J
 Time Processed: 11:35:56 PM
 Month-Day-Year Processed : 10/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

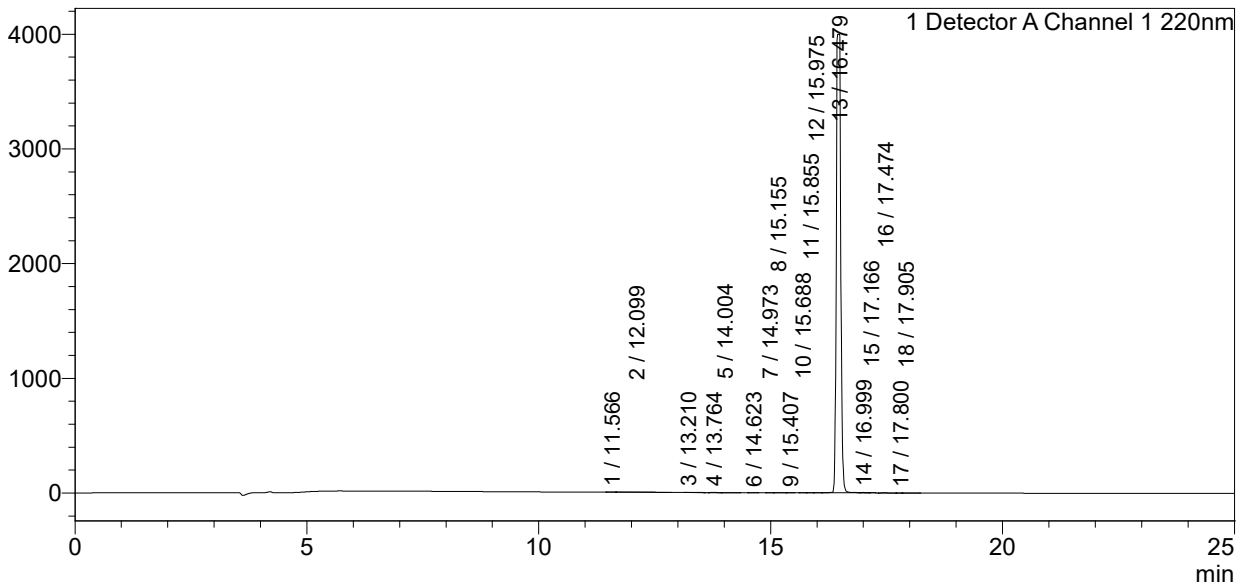

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.566	3269	303	0.012
2	12.099	110862	2900	0.416
3	13.210	3414	145	0.013
4	13.764	5346	767	0.020
5	14.004	2230	169	0.008
6	14.623	2453	389	0.009
7	14.973	1488	329	0.006
8	15.155	9859	1316	0.037
9	15.407	3388	603	0.013
10	15.688	2220	491	0.008
11	15.855	7743	1424	0.029
12	15.975	8235	1463	0.031
13	16.479	26485751	3998124	99.308
14	16.999	9642	1706	0.036

Peak#	Ret. Time	Area	Height	Area%
15	17.166	1212	324	0.005
16	17.474	7170	627	0.027
17	17.800	1303	252	0.005
18	17.905	4747	389	0.018
Total		26670330	4011721	100.000