

Sample Name :Kisspeptin-10
 Cat No. :RP20494
 Lot No. :E7602819G
 Time Processed :10:37:18 PM
 Month-Day-Year Processed :07/08/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

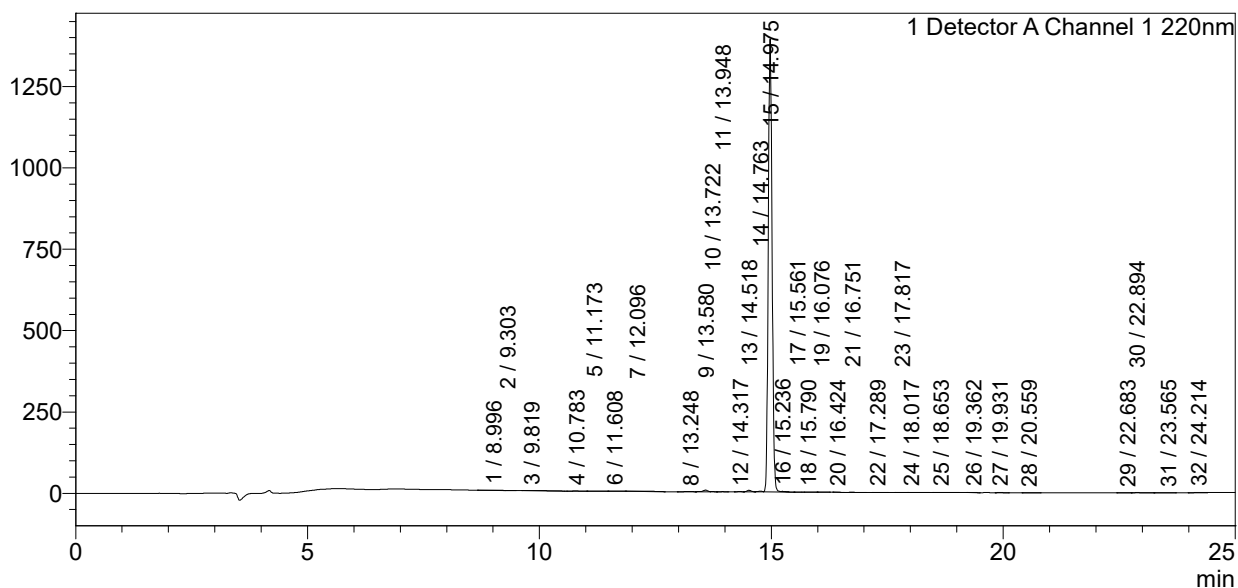

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.996	11016	597	0.135
2	9.303	1680	166	0.021
3	9.819	31027	801	0.380
4	10.783	4254	539	0.052
5	11.173	2127	162	0.026
6	11.608	4503	551	0.055
7	12.096	27161	968	0.332
8	13.248	9922	981	0.121
9	13.580	40208	5347	0.492
10	13.722	6007	1338	0.074
11	13.948	3608	601	0.044
12	14.317	7116	1126	0.087
13	14.518	32656	4883	0.400
14	14.763	17936	2307	0.220
15	14.975	7935660	1391958	97.125

Peak#	Ret. Time	Area	Height	Area%
16	15.236	2853	483	0.035
17	15.561	1997	421	0.024
18	15.790	1556	237	0.019
19	16.076	1558	175	0.019
20	16.424	1120	213	0.014
21	16.751	3748	270	0.046
22	17.289	1280	111	0.016
23	17.817	1651	145	0.020
24	18.017	2059	155	0.025
25	18.653	1404	100	0.017
26	19.362	2016	299	0.025
27	19.931	1742	296	0.021
28	20.559	1203	97	0.015
29	22.683	1403	111	0.017
30	22.894	4118	315	0.050
31	23.565	3409	179	0.042
32	24.214	2578	177	0.032
Total		8170575	1416109	100.000