

Sample Name :sgp91 ds-tat Peptide2,scrambled  
 Cat. No. : RP20436  
 Lot. No. : PE0901905  
 Time Processed : 23:53:35  
 Month-Day-Year Processed : 05/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

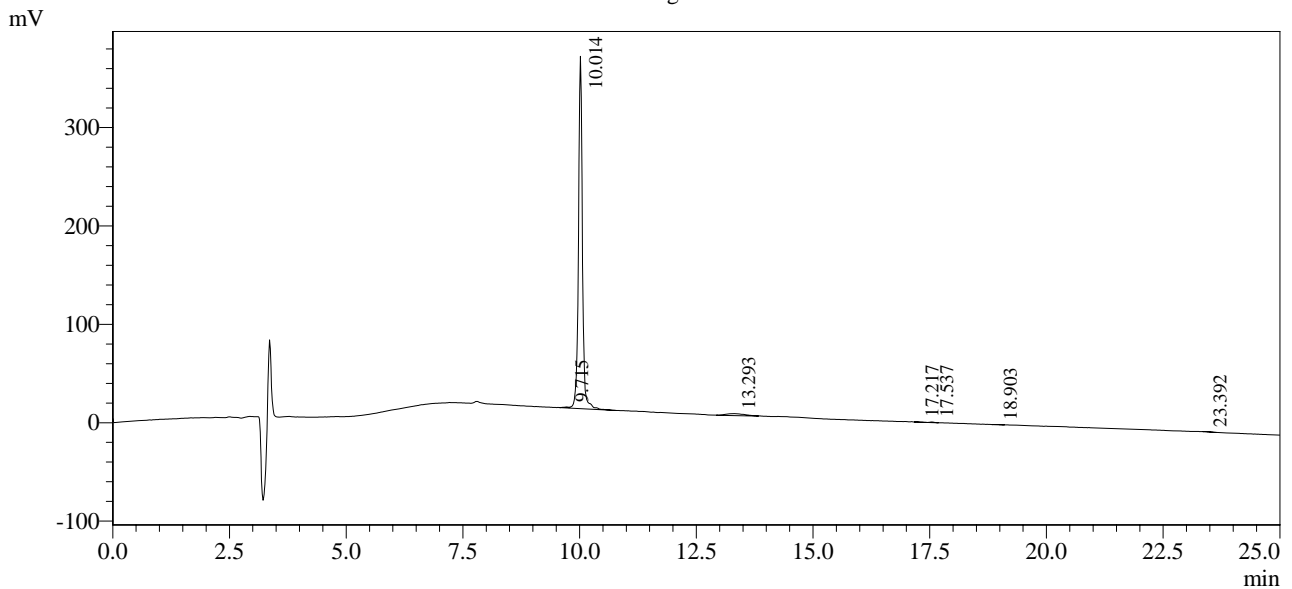

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.715	6869	940	0.316
2	10.014	2104040	358171	96.845
3	13.293	53588	1942	2.467
4	17.217	1344	227	0.062
5	17.537	3358	542	0.155
6	18.903	1302	143	0.060
7	23.392	2094	205	0.096
Total		2172594	362170	100.000