

Sample Name :Apidaecin IB  
 Cat No. :RP20409  
 Lot No. :E8363321F  
 Time Processed :6:08:47 AM  
 Month-Day-Year Processed :06/29/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

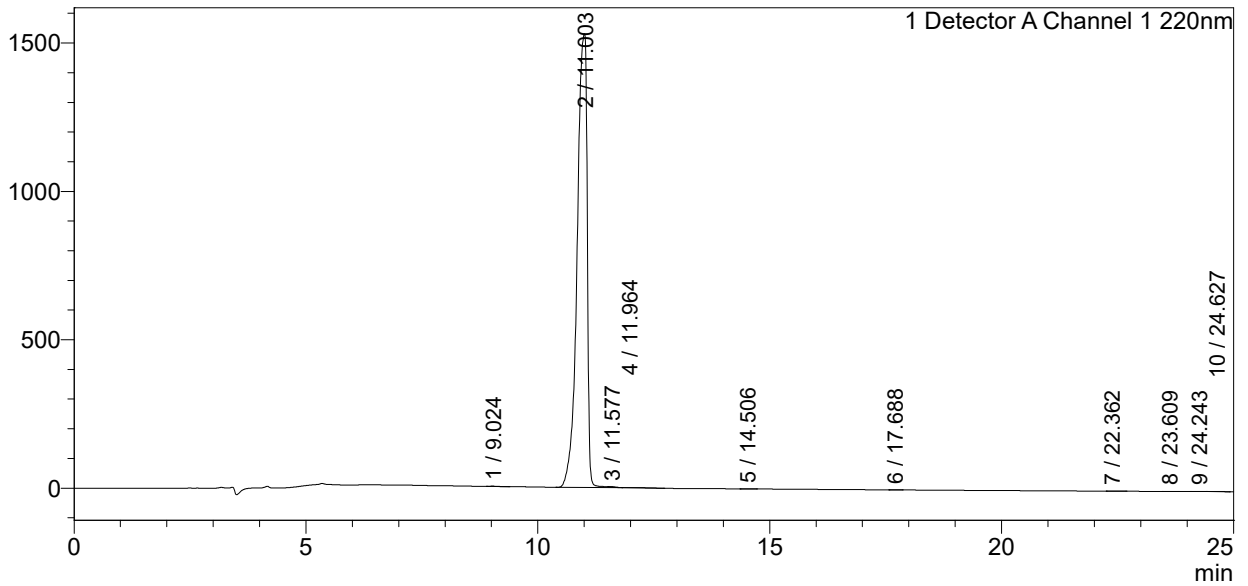

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.024	8686	1059	0.038
2	11.003	22869466	1529503	99.723
3	11.577	7070	1027	0.031
4	11.964	29058	800	0.127
5	14.506	4031	463	0.018
6	17.688	4694	617	0.020
7	22.362	1039	130	0.005
8	23.609	1568	154	0.007
9	24.243	3816	483	0.017
10	24.627	3505	277	0.015
Total		22932932	1534514	100.000