

Sample Name :OVA G4 peptide
 Cat No.: RP20398
 Lot No.: E2310120G
 Time Processed :21:05:03
 Month-Day-Year Processed :07/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

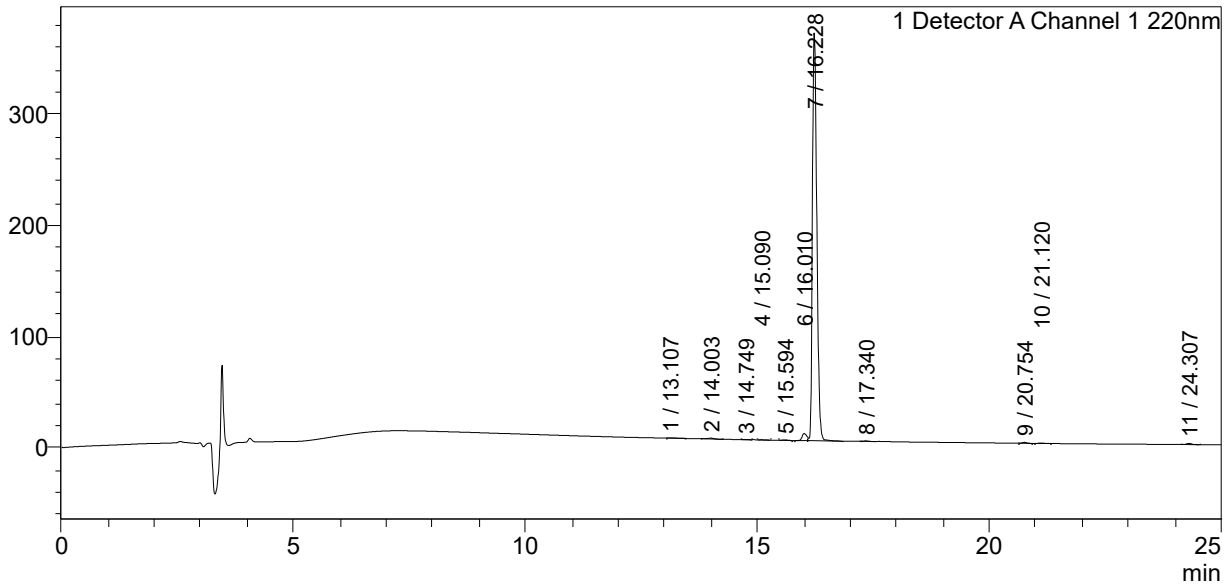

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.107	1210	90	0.048
2	14.003	7252	768	0.288
3	14.749	1094	171	0.043
4	15.090	1239	210	0.049
5	15.594	3143	510	0.125
6	16.010	47548	6419	1.889
7	16.228	2437207	367415	96.838
8	17.340	2813	430	0.112
9	20.754	5312	879	0.211
10	21.120	2368	337	0.094
11	24.307	7610	983	0.302
Total		2516796	378212	100.000