

Sample Name :p5 Ligand for Dnak and and Dnal
 Cat. No. :RP20327
 Lot. No. :PE7231710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

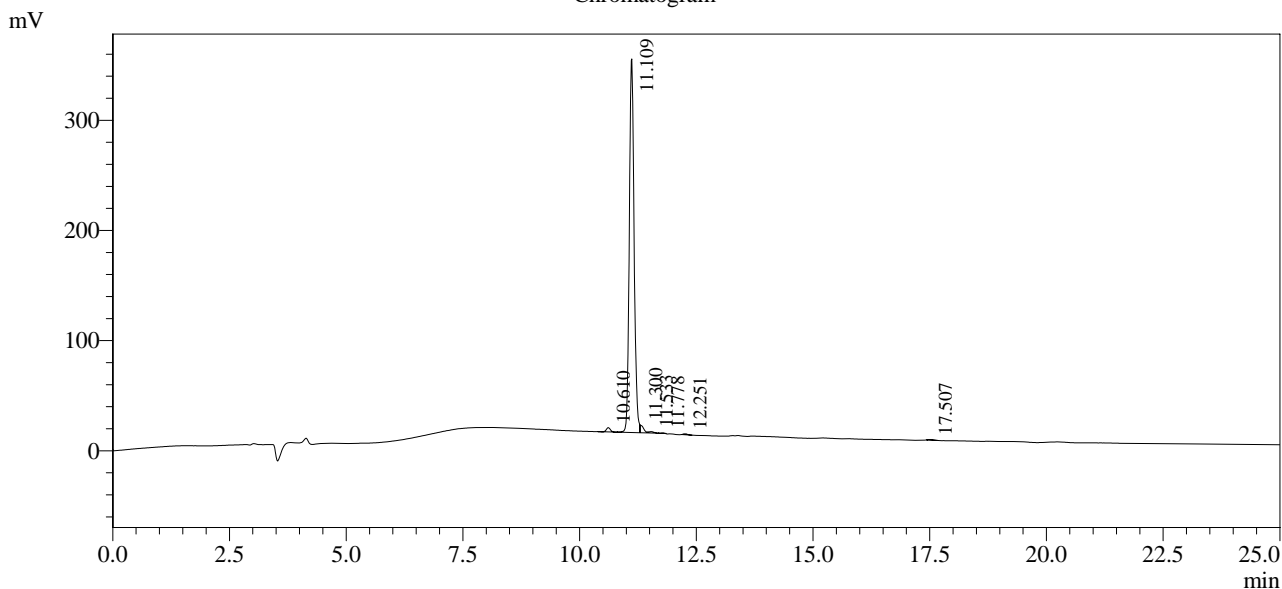

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.610	21787	3864	0.873
2	11.109	2418589	339195	96.866
3	11.300	36216	6887	1.450
4	11.533	9570	1275	0.383
5	11.778	1537	363	0.062
6	12.251	5574	991	0.223
7	17.507	3576	490	0.143
Total		2496850	353065	100.000