

Sample Name :EGFRvIII peptide (PEPvIII)
 Cat No. : RP20356
 Lot No. : E0324820B
 Time Processed : 19:59:54
 Month-Day-Year Processed : 02/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

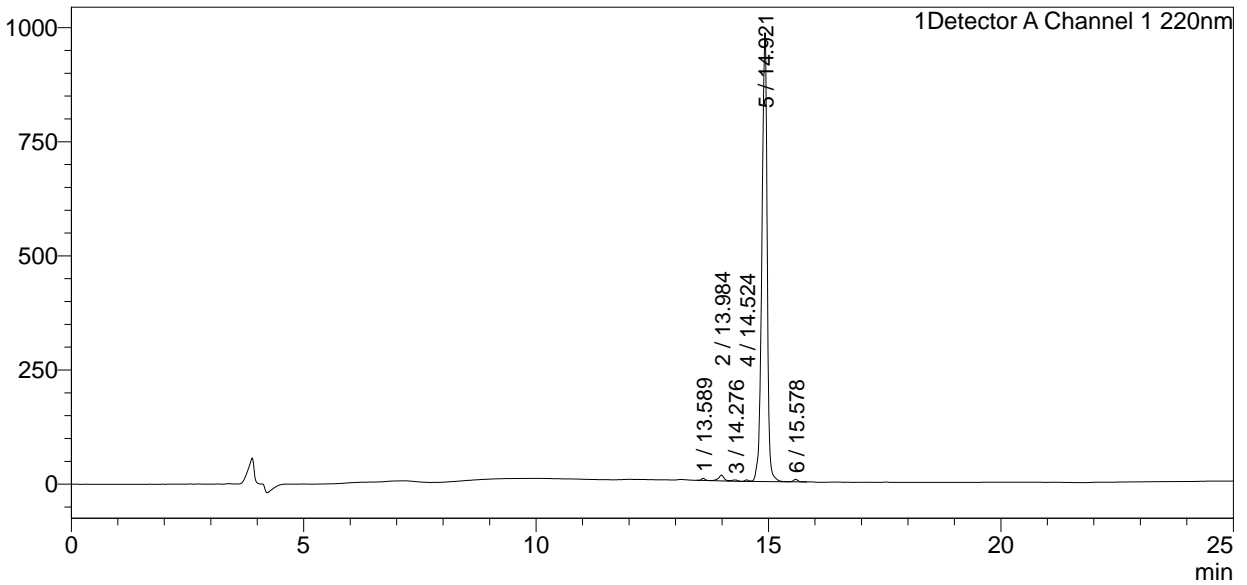

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.589	26916	4777	0.334
2	13.984	104049	12809	1.292
3	14.276	24939	2778	0.310
4	14.524	18498	3357	0.230
5	14.921	7839796	982857	97.326
6	15.578	40964	5684	0.509
Total		8055161	1012261	100.000