

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No. :RP11110
 Lot No. :E5657120C
 Time Processed : 12:52:31
 Month-Day-Year Processed : 03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

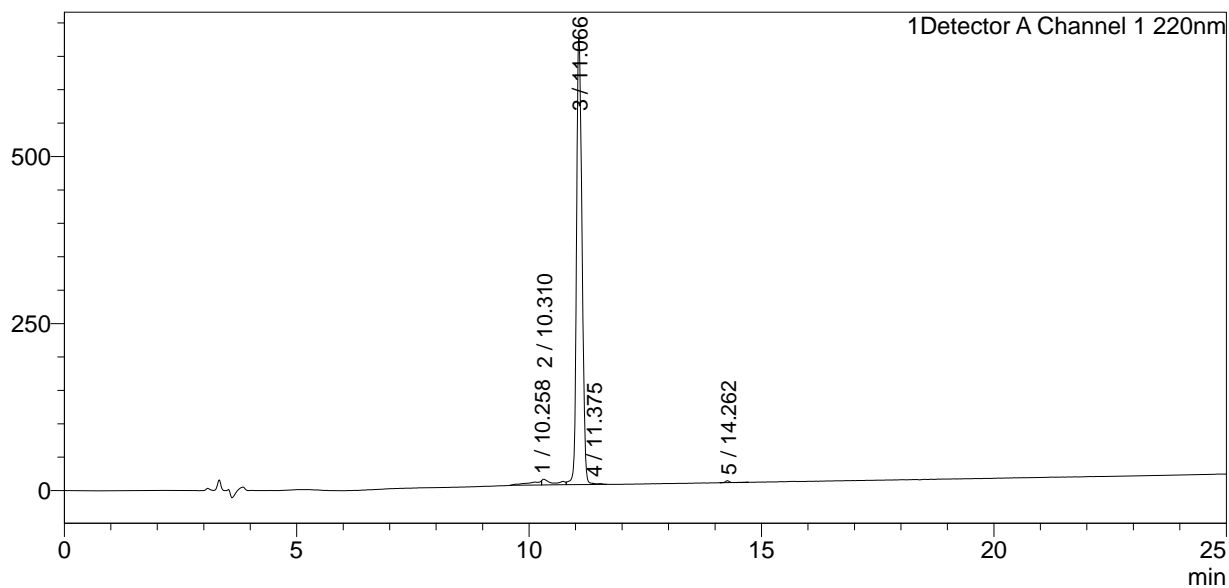

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.258	112671	5718	1.952
2	10.310	145132	8699	2.514
3	11.066	5484689	668743	95.025
4	11.375	14200	1711	0.246
5	14.262	15162	2941	0.263
Total		5771855	687812	100.000