

Sample Name : Uty HY Peptide (246-254)
 Cat. No. : RP20261
 Lot. No. : E9626619L
 Time Processed :2:36:50
 Month-Day-Year Processed :12/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

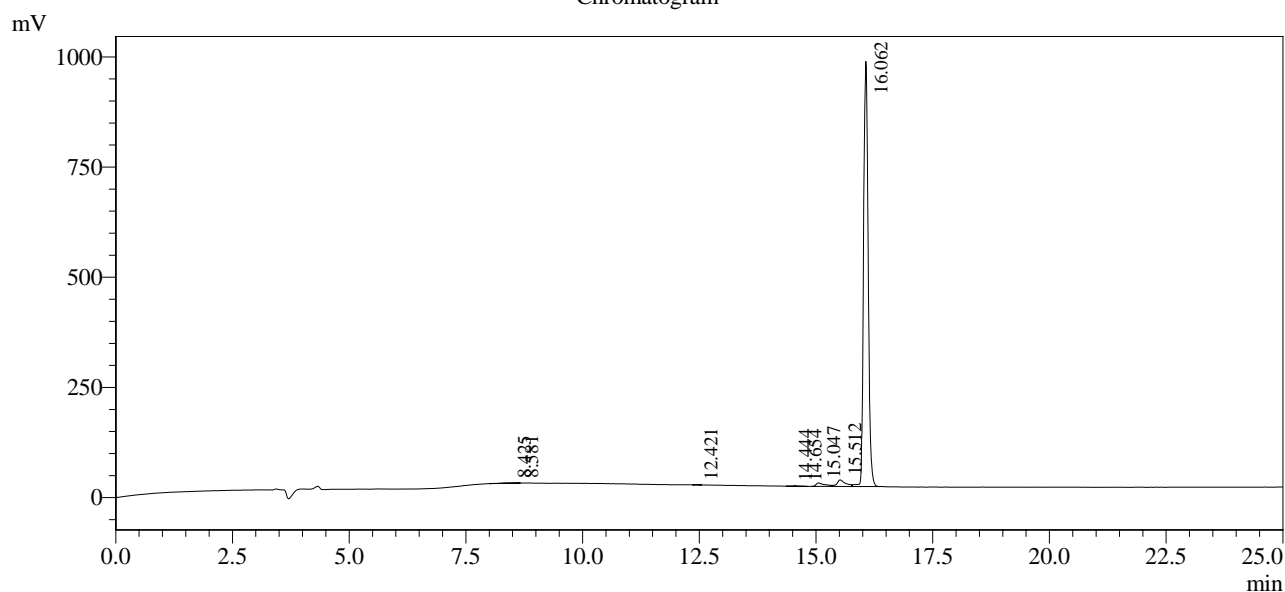

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.425	10386	507	0.149
2	8.581	2916	392	0.042
3	12.421	2736	501	0.039
4	14.444	1651	335	0.024
5	14.654	3450	463	0.050
6	15.047	103356	7646	1.486
7	15.512	183967	14949	2.644
8	16.062	6649047	964969	95.566
Total		6957510	989761	100.000