

Sample Name: GRGDSP  
 Cat No. :RP20255  
 Lot No. :E8882620I  
 Time Processed: 10:31:30 AM  
 Month-Day-Year Processed :09/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

<Chromatogram>

mV

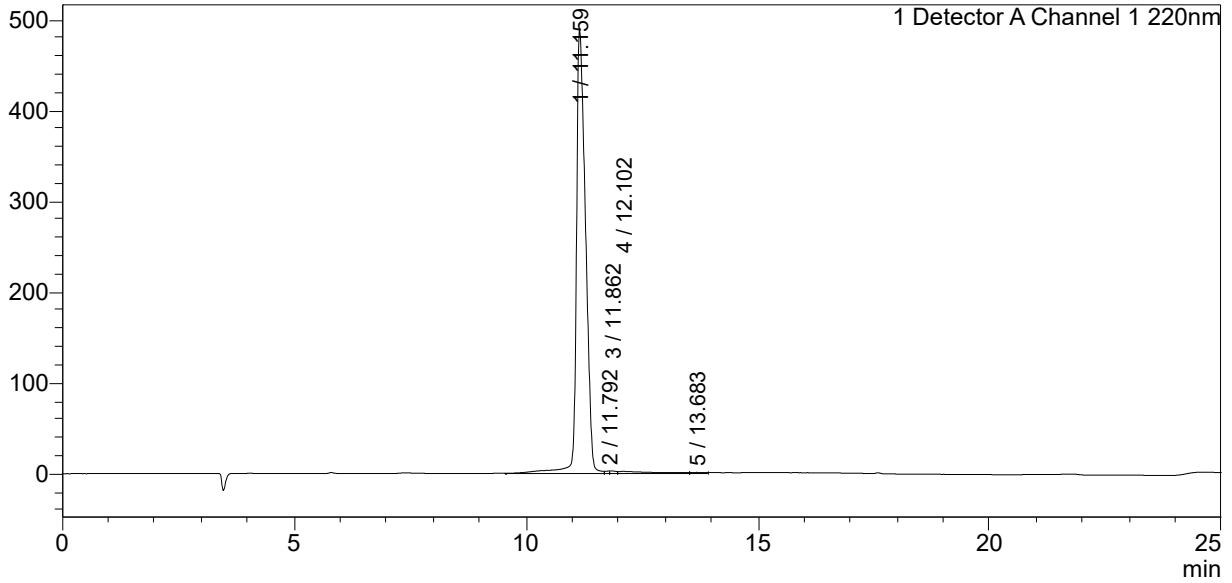

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.159	6735642	489141	96.883
2	11.792	21347	2769	0.307
3	11.862	25581	2814	0.368
4	12.102	144861	2526	2.084
5	13.683	24889	1326	0.358
Total		6952319	498576	100.000