

Sample Name : Gly-Arg-Gly-Asp-Asn-Pro
 Cat. No. : RP10847
 Lot. No. : E7226820B
 Time Processed : 9:41:33
 Month-Day-Year Processed : 02/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

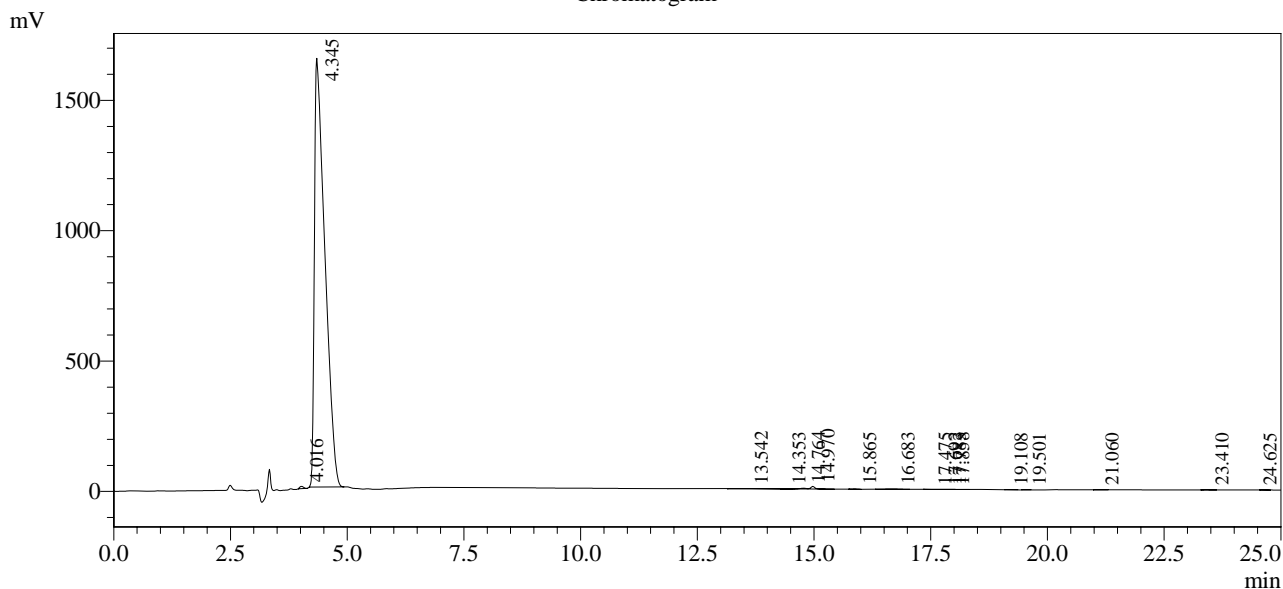

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.016	47871	8533	0.184
2	4.345	25707422	1644554	99.017
3	13.542	53026	2070	0.204
4	14.353	1384	224	0.005
5	14.764	31546	3070	0.122
6	14.970	66735	10028	0.257
7	15.865	4045	602	0.016
8	16.683	25913	1303	0.100
9	17.475	1036	180	0.004
10	17.692	5341	499	0.021
11	17.783	2588	495	0.010
12	17.858	6190	488	0.024
13	19.108	1115	137	0.004
14	19.501	1108	164	0.004
15	21.060	1176	135	0.005
16	23.410	4699	509	0.018
17	24.625	1310	160	0.005
Total		25962507	1673149	100.000