

Sample Name :Moth Cytochrome C (MCC) (88-103)
 Cat No. :RP12808
 Lot No. :E4783419J
 Time Processed :7:59:38 AM
 Month-Day-Year Processed :10/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

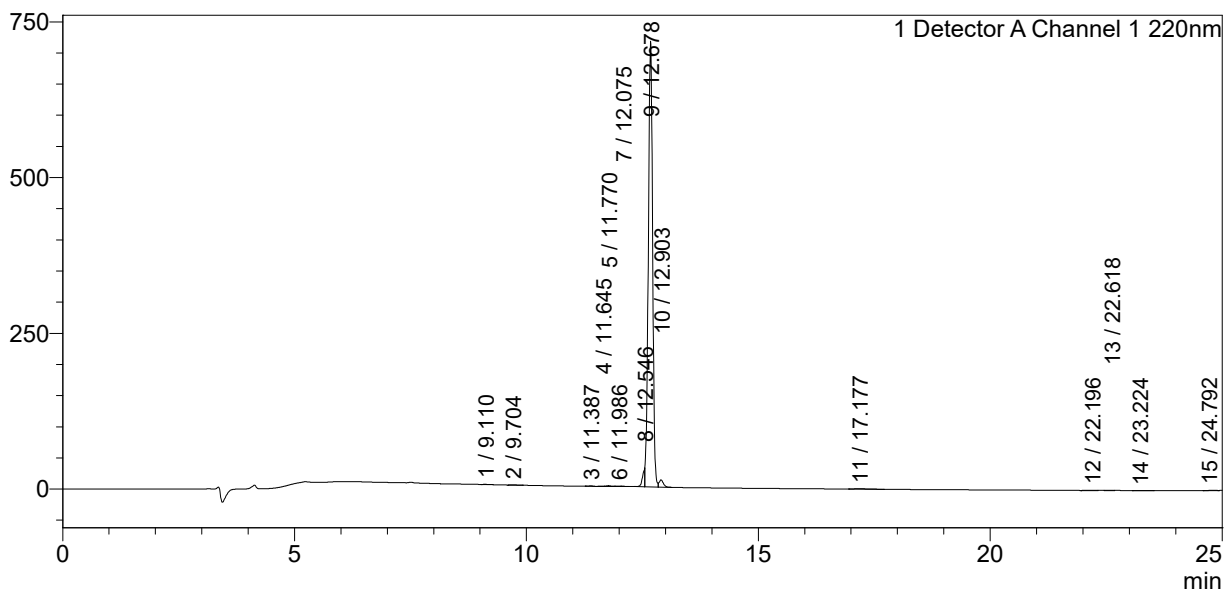

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.110	1845	294	0.038
2	9.704	4321	621	0.090
3	11.387	4099	763	0.085
4	11.645	3311	503	0.069
5	11.770	8281	1152	0.172
6	11.986	1439	200	0.030
7	12.075	1012	194	0.021
8	12.546	100748	27166	2.091
9	12.678	4599952	715622	95.477
10	12.903	71865	11545	1.492
11	17.177	13666	754	0.284
12	22.196	2277	146	0.047
13	22.618	1324	113	0.027
14	23.224	1519	98	0.032
15	24.792	2194	286	0.046

Peak#	Ret. Time	Area	Height	Area%
Total		4817852	759460	100.000