

Sample Name :β-MSH, human
Cat. No. : RP10648
Lot. No. : PE3871811
Time Processed : 20:17:55
Month-Day-Year Processed : 11/14/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

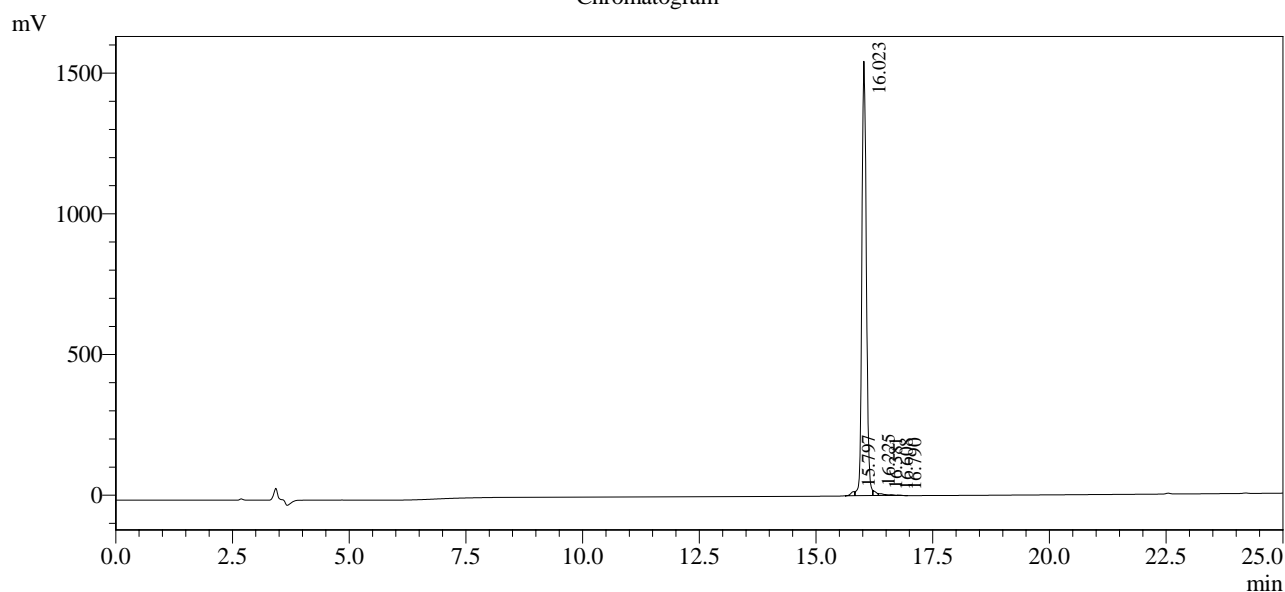

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.797	88302	14506	0.835
2	16.023	10336923	1543835	97.738
3	16.225	82531	17410	0.780
4	16.381	53128	6331	0.502
5	16.608	11154	1738	0.105
6	16.790	4129	869	0.039
Total		10576167	1584690	100.000