

Sample Name :[Glu1]-Fibrinopeptide B
 Cat. No. :RP20439
 Lot. No. :E3923119F
 Time Processed : 11:26:54
 Month-Day-Year Processed :06/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

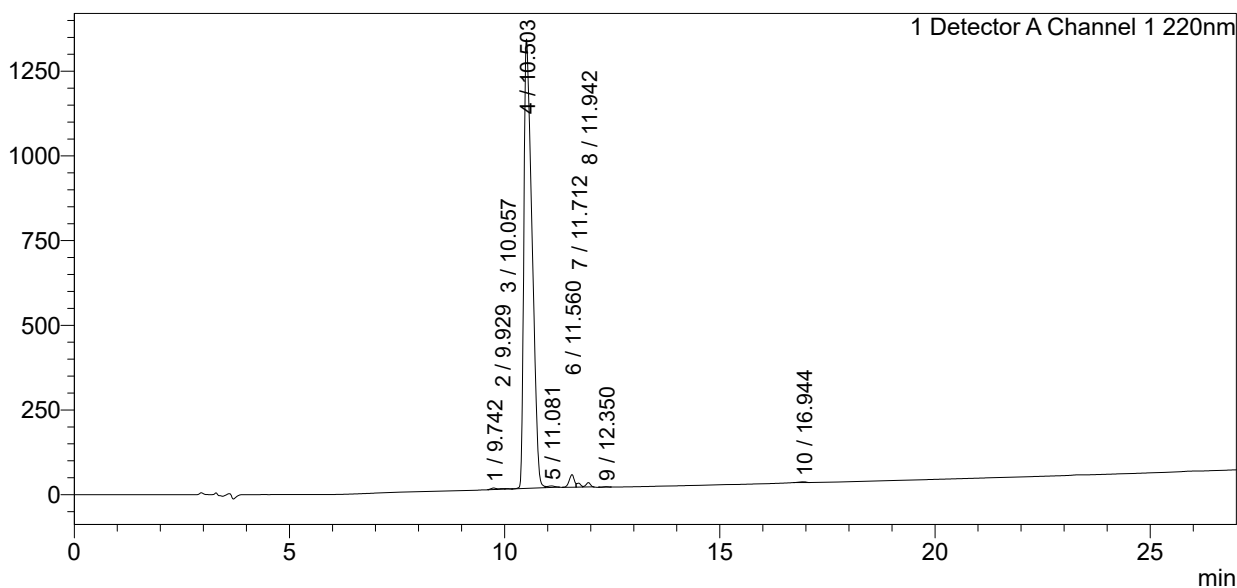

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.742	33865	4401	0.187
2	9.929	18987	1896	0.105
3	10.057	8589	1495	0.047
4	10.503	17502746	1326471	96.561
5	11.081	55255	4455	0.305
6	11.560	303198	37288	1.673
7	11.712	75717	11634	0.418
8	11.942	91563	13147	0.505
9	12.350	8905	1277	0.049
10	16.944	27299	2425	0.151
Total		18126123	1404490	100.000