

Sample Name :p5 Ligand for Dnak and and Dnal  
 Cat. No. : RP20327  
 Lot. No. :PE9171706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

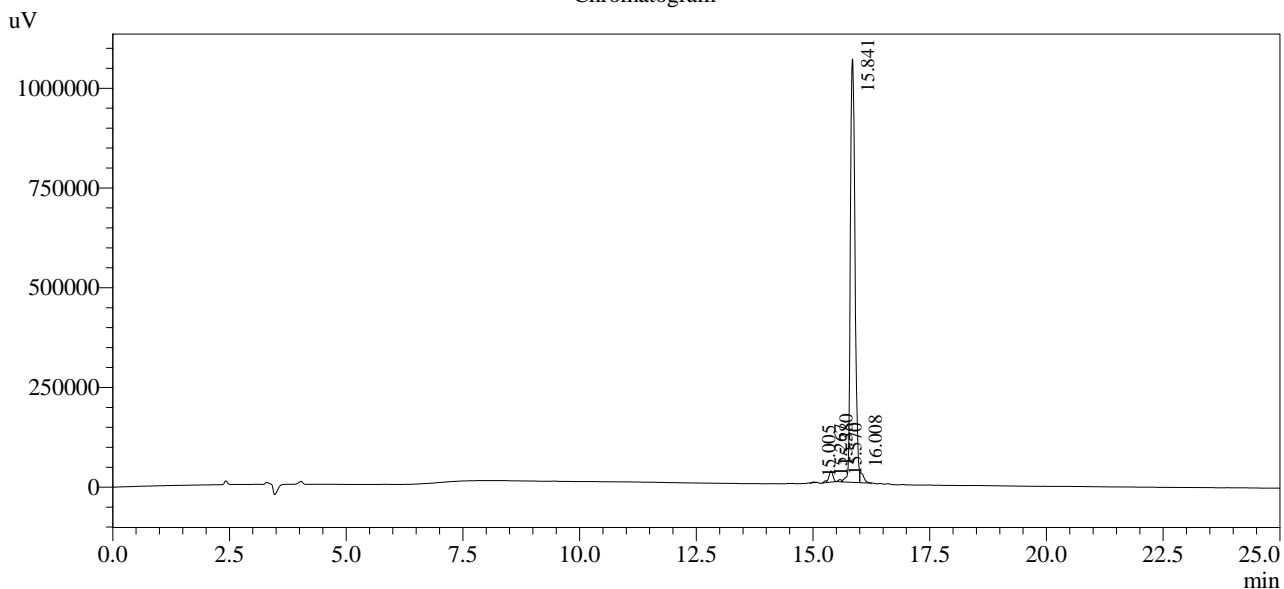

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.005	7148	1746	0.093
2	15.267	17975	4538	0.233
3	15.380	163118	28225	2.115
4	15.570	26840	5068	0.348
5	15.841	7349543	1061517	95.309
6	16.008	146619	26240	1.901
Total		7711242	1127334	100.000