

Sample Name : Indolicidin
 Cat. No. : RP11242
 Lot. No. : PE0501707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

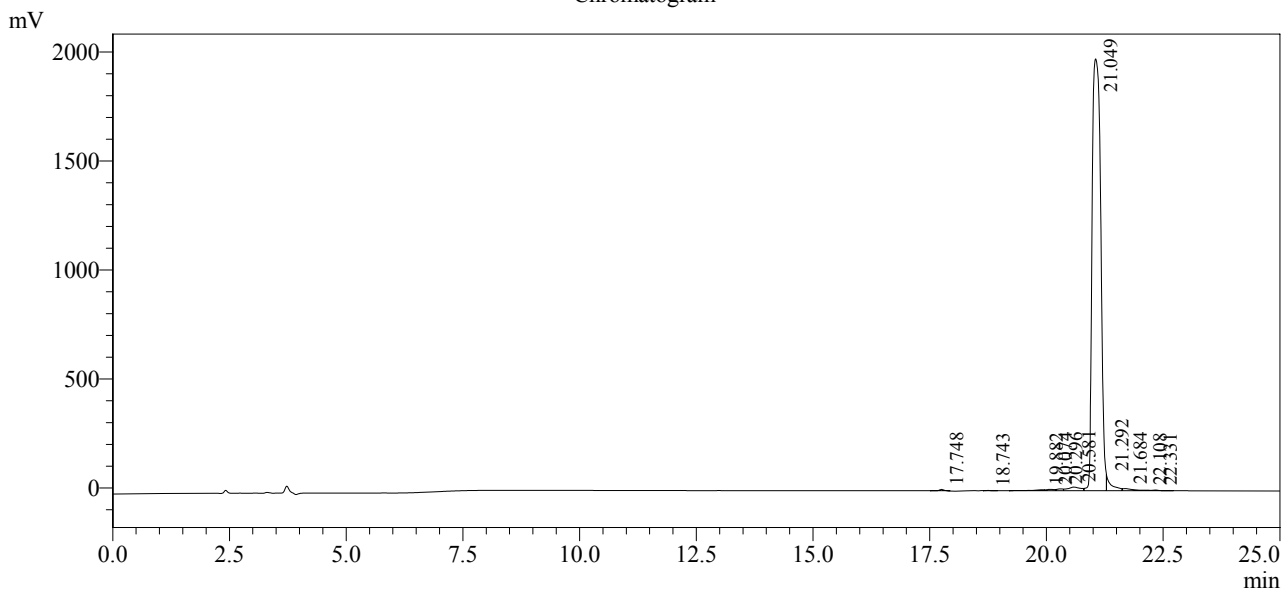

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.748	35679	5801	0.134
2	18.743	8203	1373	0.031
3	19.882	67907	4196	0.256
4	20.074	74459	6009	0.280
5	20.296	73945	8246	0.278
6	20.581	308482	16534	1.161
7	21.049	25319054	1981171	95.325
8	21.292	474103	66794	1.785
9	21.684	135029	9520	0.508
10	22.108	34545	2672	0.130
11	22.331	29310	3116	0.110
Total		26560718	2105432	100.000