


Mass Spectrum

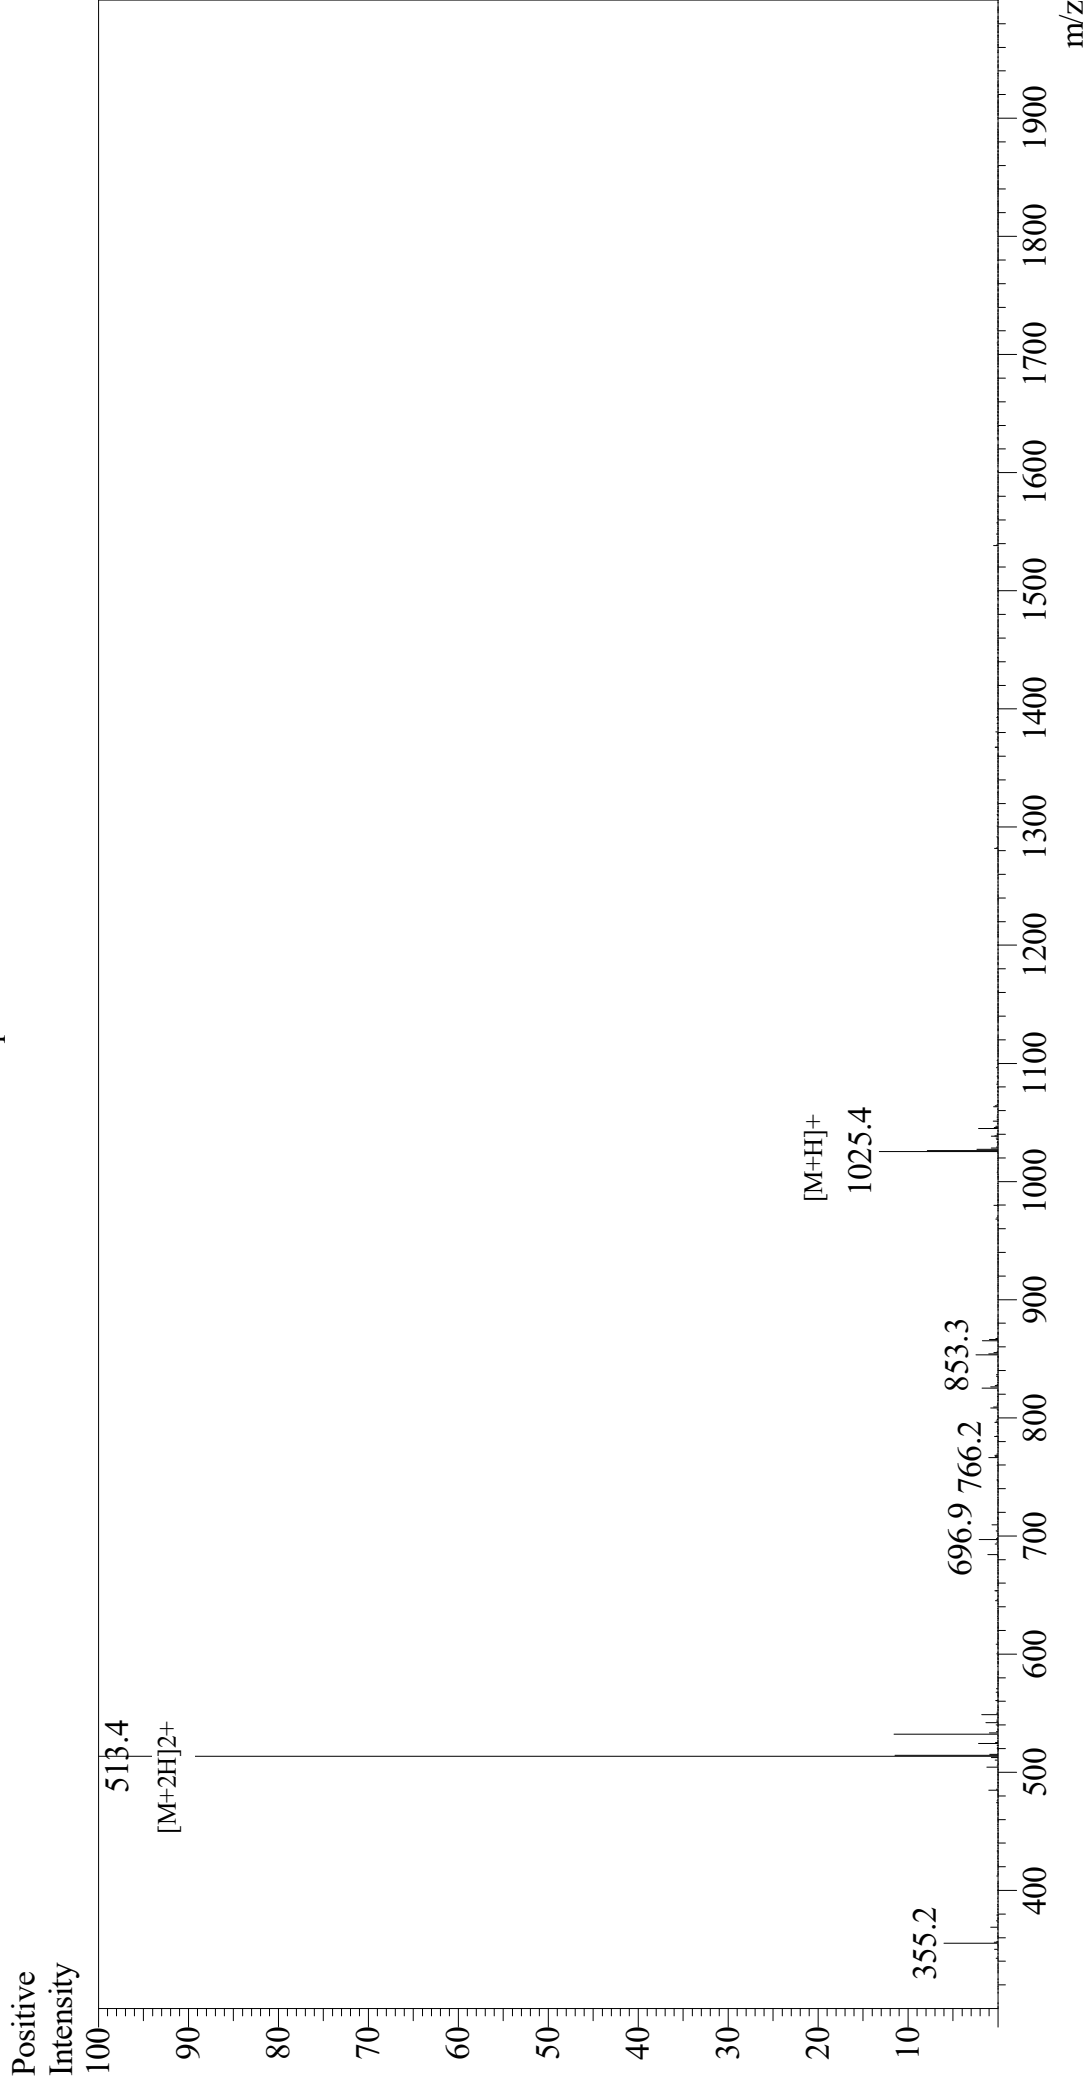

Sample Information
 Month-Day Processed : 11/11/21
 Time Processed : 8:49:36 PM
 Injection Volume : 0.4
 Sample Name : RGD
 Cat No. : RP20297
 Lot No. : E6980621K
 Theoretical MW : 1025.06
 Observed MW : 1024.8

Interface : ESI
 Nebulizing Gas Flow : 1.5 L/min
 CDL Temp : 250
 Block Temp : 200
 Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H2O/50% MeOH