

Sample Name : Kisspeptin-10
 Cat. No. : RP20494
 Lot. No. : PE0261801

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

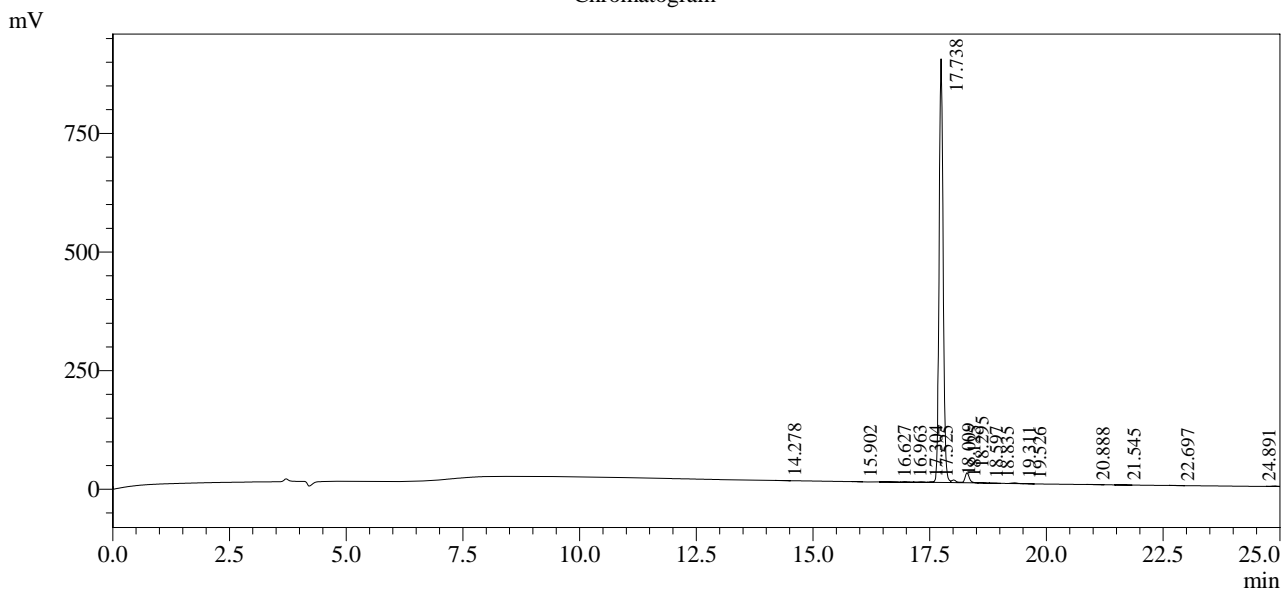

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.278	2219	250	0.039
2	15.902	1063	198	0.019
3	16.627	7679	711	0.136
4	16.963	6198	847	0.110
5	17.304	6396	727	0.113
6	17.525	5885	1166	0.104
7	17.738	5406369	892840	95.852
8	18.009	36329	5570	0.644
9	18.125	4119	1128	0.073
10	18.295	132940	20976	2.357
11	18.597	2374	345	0.042
12	18.835	2725	298	0.048
13	19.311	12586	1403	0.223
14	19.526	1002	113	0.018
15	20.888	1289	53	0.023
16	21.545	1249	165	0.022
17	22.697	1760	153	0.031
18	24.891	8149	1008	0.144
Total		5640329	927951	100.000