

Sample Name :PAR-4AgonistPeptide,amide

Cat. No. : RP11529

Lot. No. : PE3491904

Time Processed : 9:10:16

Month-Day-Year Processed : 04/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

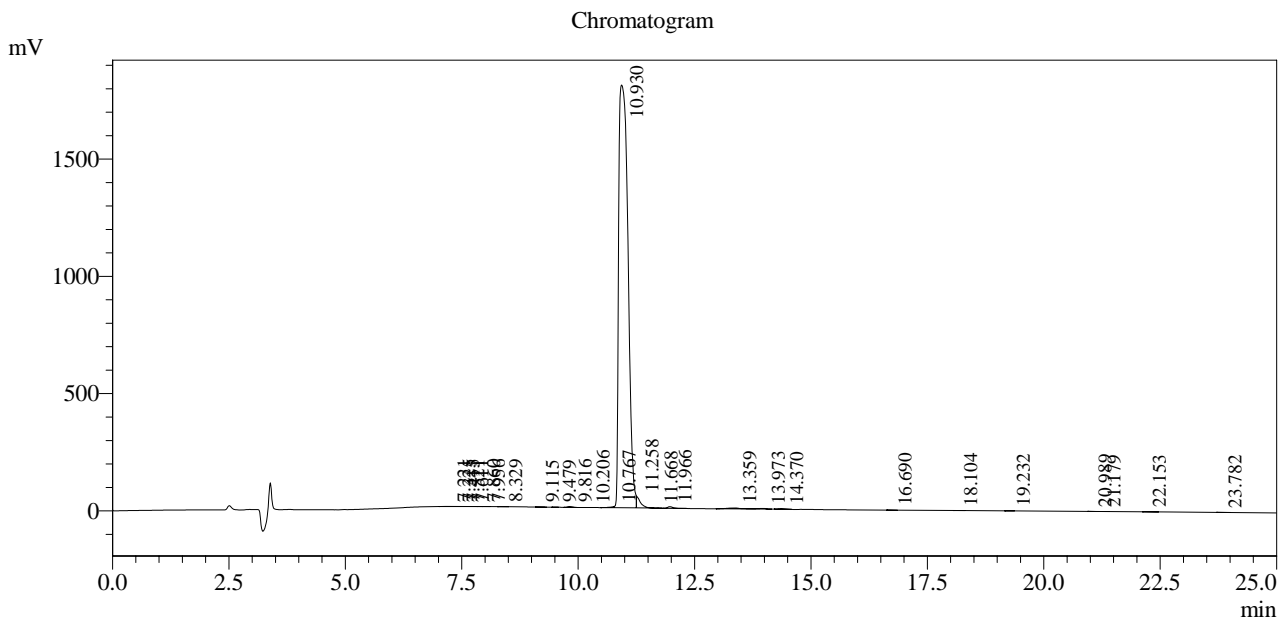

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.221	7674	847	0.030
2	7.325	6195	930	0.024
3	7.415	3884	1002	0.015
4	7.521	7606	1035	0.030
5	7.611	8897	856	0.035
6	7.860	2483	452	0.010
7	7.956	1893	322	0.007
8	8.329	4709	674	0.018
9	9.115	1574	186	0.006
10	9.479	1160	254	0.005
11	9.816	25830	3508	0.101
12	10.206	1830	324	0.007
13	10.767	30672	4797	0.120
14	10.930	24974821	1802637	97.637
15	11.258	284929	48722	1.114
16	11.668	3195	489	0.012
17	11.966	58641	7070	0.229
18	13.359	88588	3929	0.346
19	13.973	38767	2921	0.152
20	14.370	12917	1742	0.050
21	16.690	1834	275	0.007
22	18.104	1969	149	0.008

Peak#	Ret. Time	Area	Height	Area %
23	19.232	1503	242	0.006
24	20.989	1097	186	0.004
25	21.179	1158	121	0.005
26	22.153	2052	213	0.008
27	23.782	3449	410	0.013
Total		25579327	1884291	100.000