

Sample Name : GnRH-I
 Cat. No. : RP20303
 Lot. No. : E1108819I
 Time Processed :12:26:44
 Month-Day-Year Processed :09/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

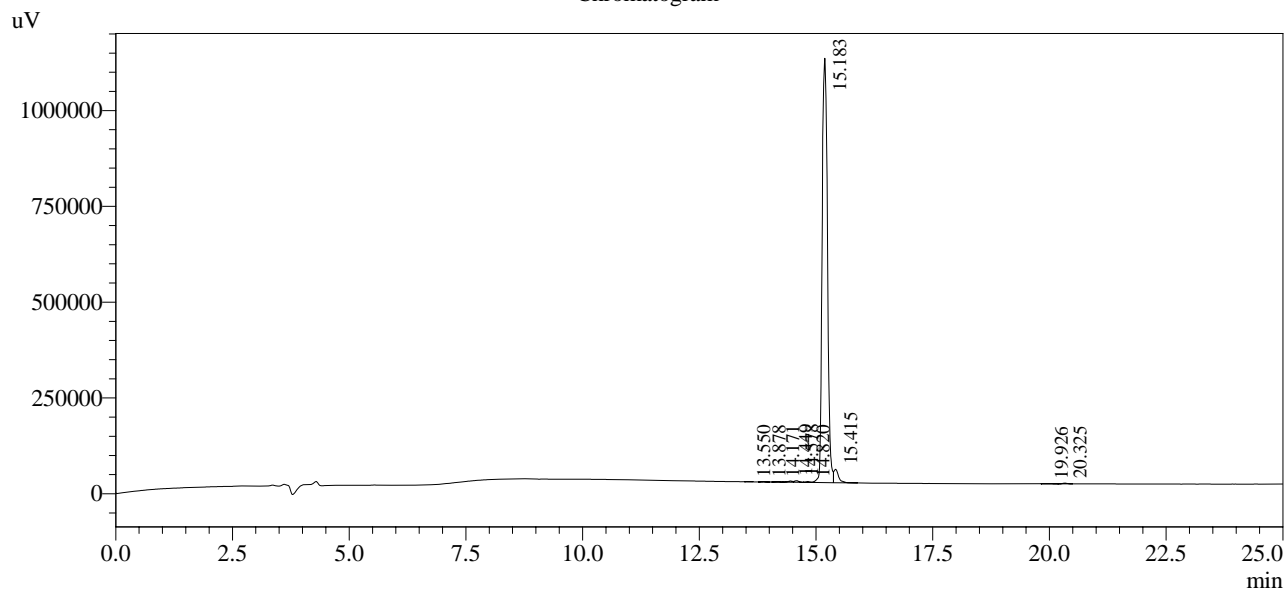

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.550	1733	365	0.019
2	13.878	5990	945	0.065
3	14.171	6500	1226	0.071
4	14.449	22886	3051	0.249
5	14.578	25012	4133	0.272
6	14.820	10622	1864	0.116
7	15.183	8860614	1107345	96.405
8	15.415	239915	35074	2.610
9	19.926	4799	399	0.052
10	20.325	12977	1938	0.141
Total		9191047	1156341	100.000