

Sample Name : Apidaecin IB
 Cat. No. : RP20409
 Lot. No. : E7291619H
 Time Processed : 8:24:17
 Month-Day-Year Processed : 08/31/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

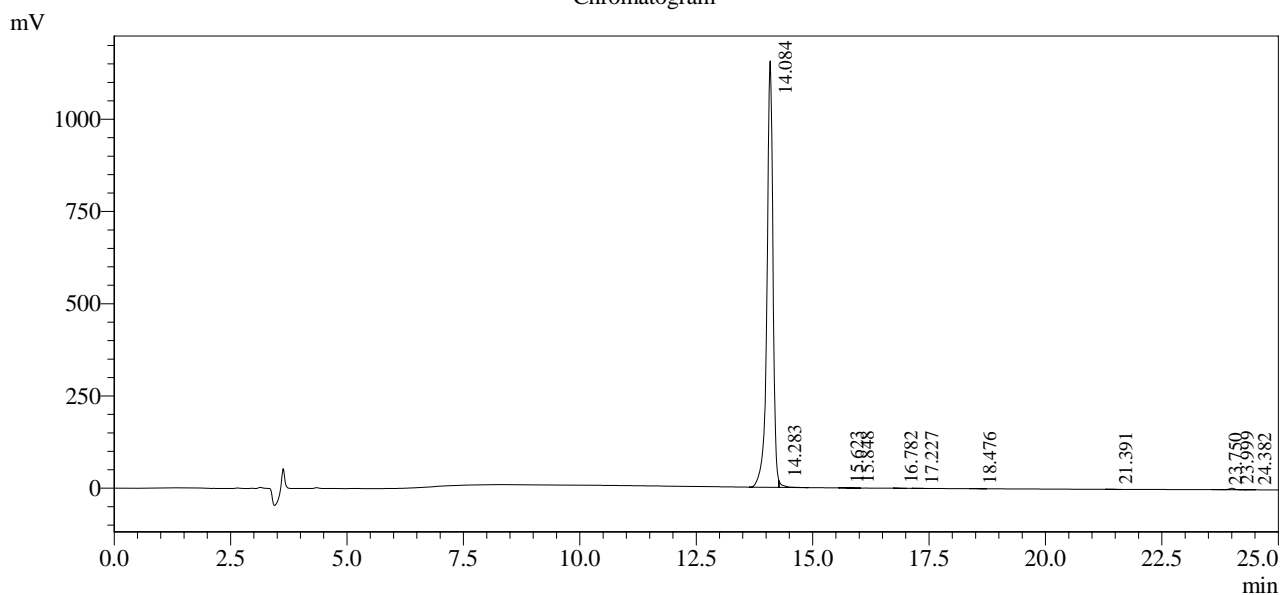

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.084	10338453	1155731	98.768
2	14.283	80012	15413	0.764
3	15.623	1391	214	0.013
4	15.848	1122	200	0.011
5	16.782	1031	88	0.010
6	17.227	3738	363	0.036
7	18.476	2153	253	0.021
8	21.391	1971	295	0.019
9	23.750	3034	251	0.029
10	23.999	32578	4025	0.311
11	24.382	1951	305	0.019
Total		10467433	1177137	100.000