


# Mass Spectrum

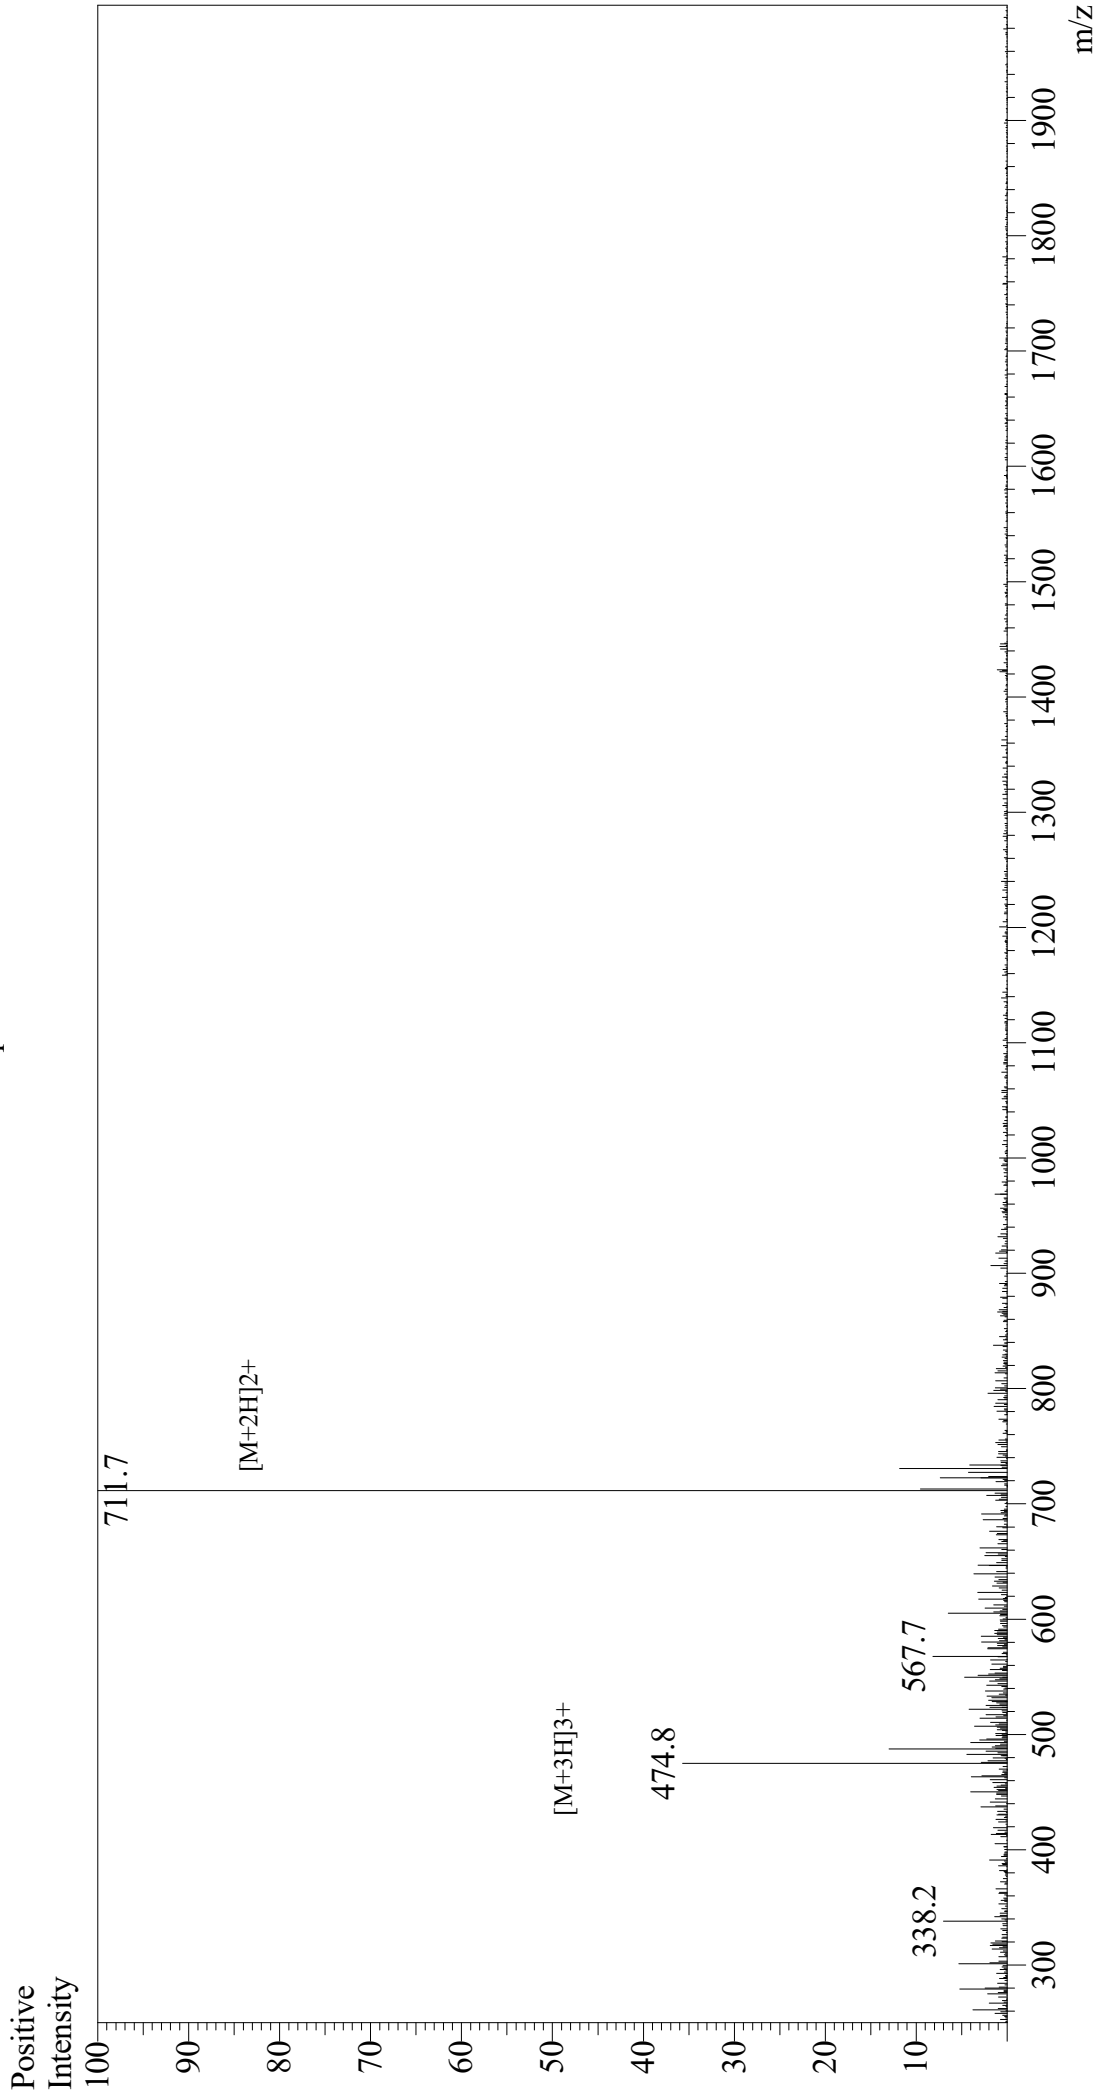

Sample Information  
Month-Day Processed : 11/26/20  
Time Processed : 11:50:50 AM  
Injection Volume : 0.3  
Sample Name : Mas7  
Cat No. : RP10602  
Lot No. : E5881320K  
Theoretical MW : 1421.81  
Observed MW : 1421.4

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH